




2022-01-11

Anions

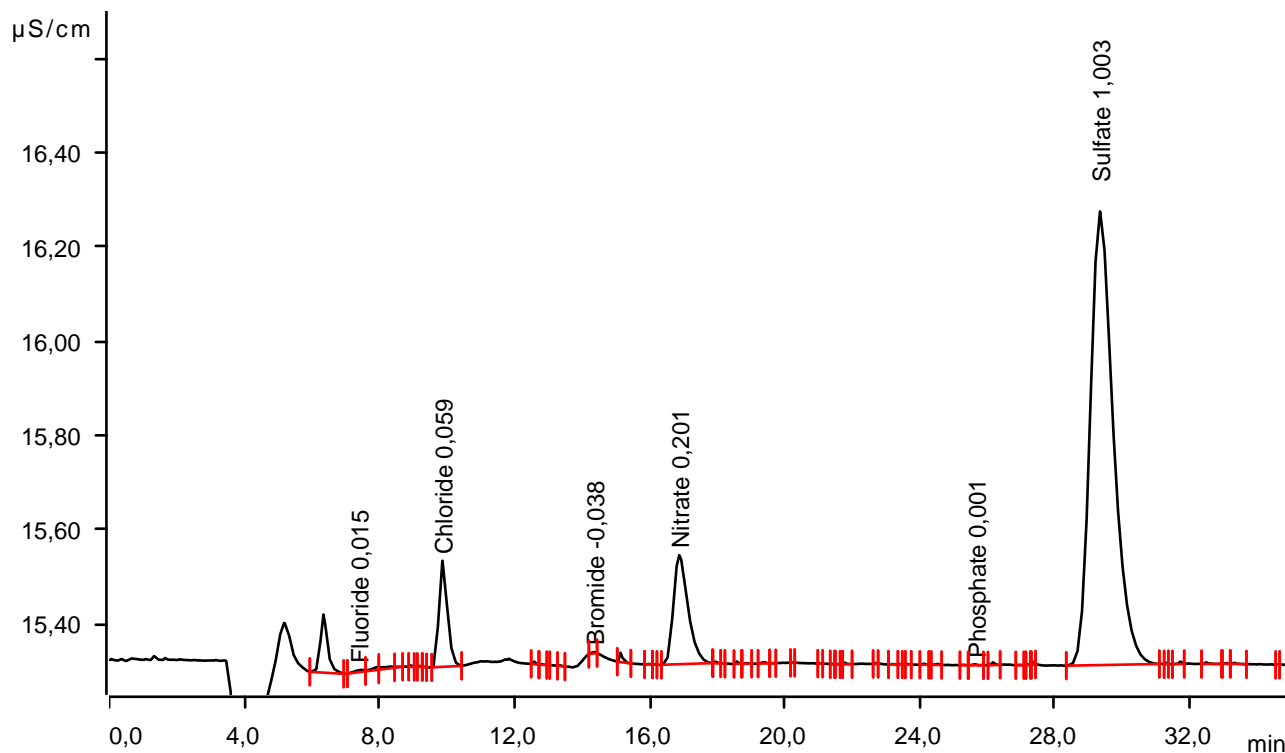

Component name	Retention time	Height	Area	Concentration
	min	μS/cm	(μS/cm) x min	ppm
Fluoride	7,44	0,004	0,001	0,015
Chloride	9,87	0,225	0,065	0,059
Bromide	14,36	0,003	0,000	-0,038
Nitrate	16,88	0,232	0,116	0,201
Phosphate	25,60	0,002	0,000	0,001
Sulfate	29,34	0,963	0,765	1,003

Sample data

Ident 2B Santanna 2
Sample type Sample
Position 12
Injections 1
Injection counter 1
Volume 100 μL
Dilution 1
Sample amount 1
Info 1