




Anions

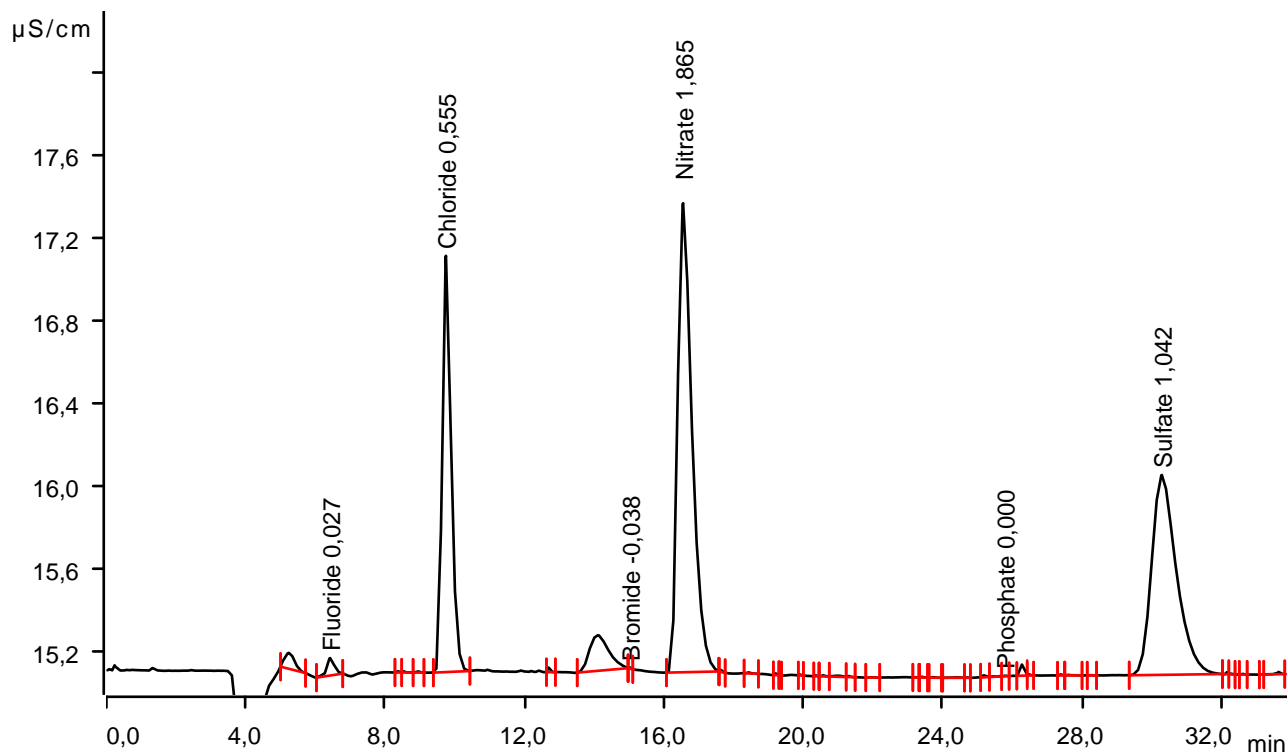

Component name	Retention time	Height	Area	Concentration
	min	µS/cm	(µS/cm) x min	ppm
Fluoride	6,42	0,084	0,021	0,027
Chloride	9,74	2,012	0,593	0,555
Bromide	15,01	0,006	0,000	-0,038
Nitrate	16,55	2,266	1,082	1,865
Phosphate	25,77	0,003	0,000	0,000
Sulfate	30,28	0,966	0,795	1,042

Sample data

Ident 8A san benedetto 1
Sample type Sample
Position 20
Injections 1
Injection counter 1
Volume 100 µL
Dilution 1
Sample amount 1
Info 1