

MRS

Magnetic Resonance Spectroscopy



In vivo biochemistry

The background is a solid blue color. In the lower right quadrant, there are several sets of concentric, light blue circles that resemble ripples on water. These circles are of varying sizes and are arranged in a way that suggests movement or a field of activity.

Chemical shift




Chemical shift and MR spectrum

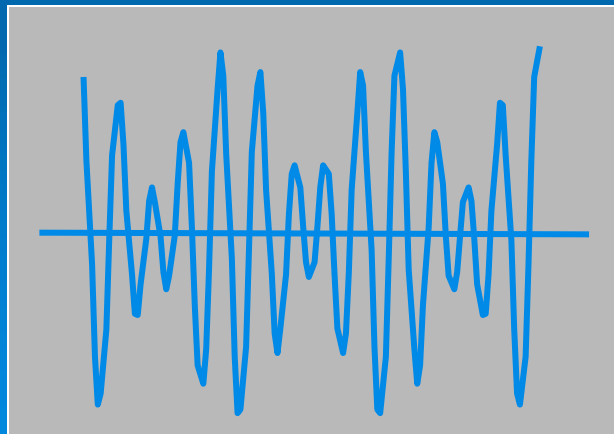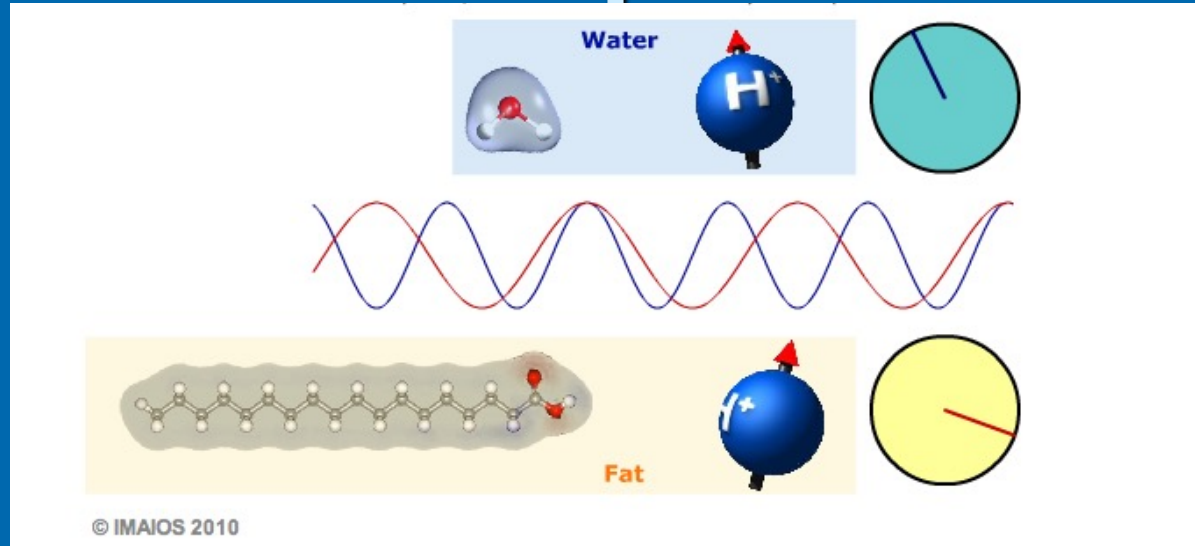



Received Signal

Fourier
Transform

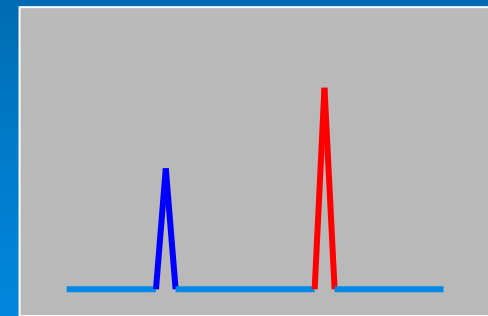


Image

^1H NMR spectra

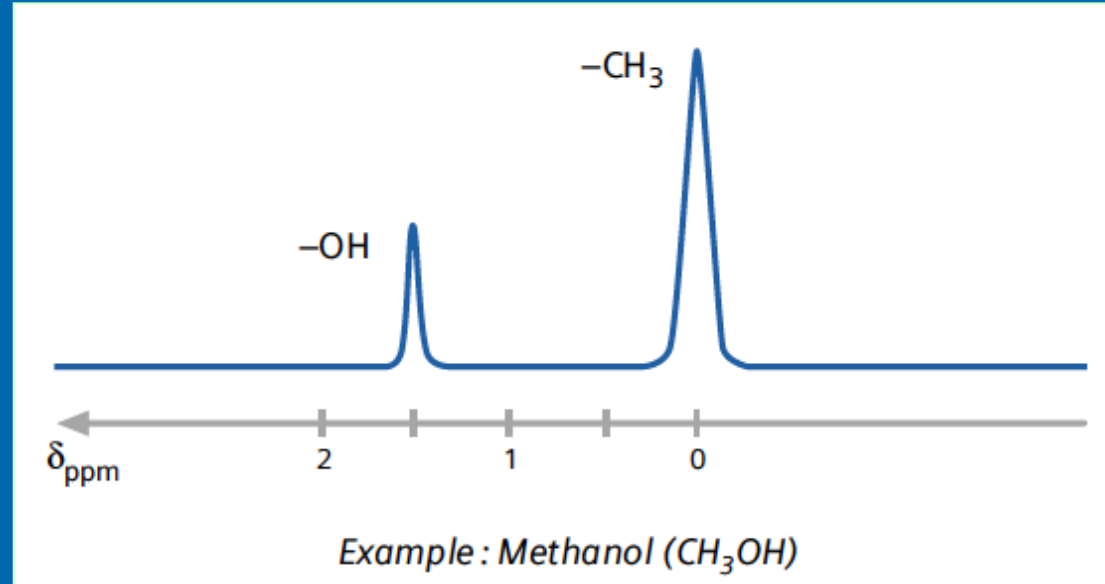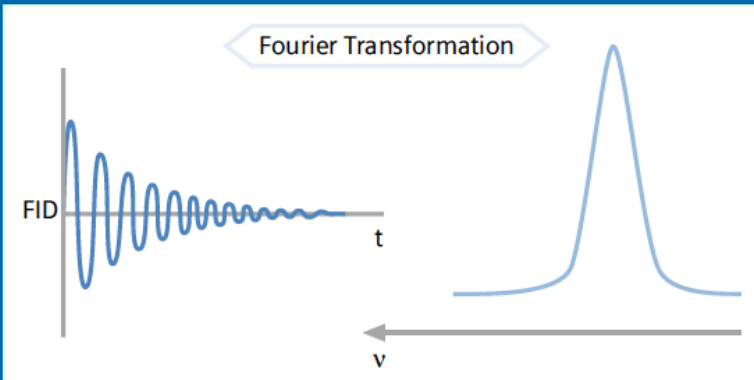

- ✓ Peaks pattern is footprint of molecules
- ✓ Peak area is proportional to the number of ^1H nuclei

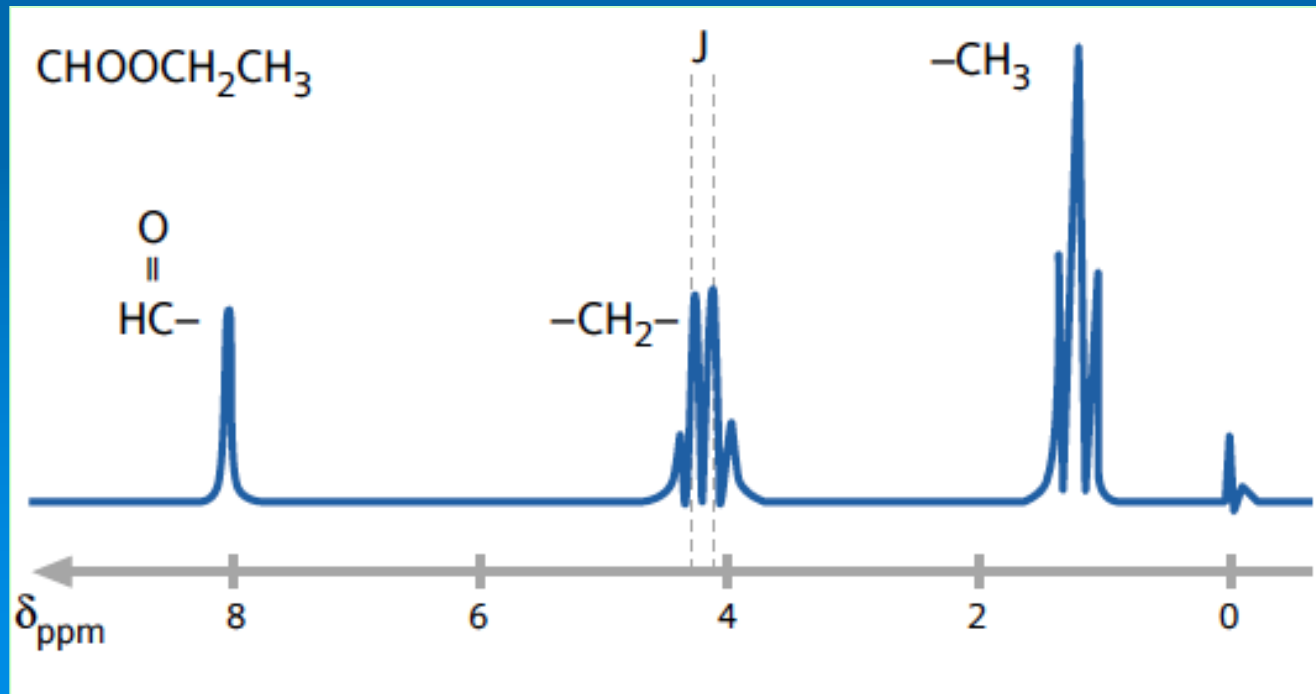

Proton spectroscopy


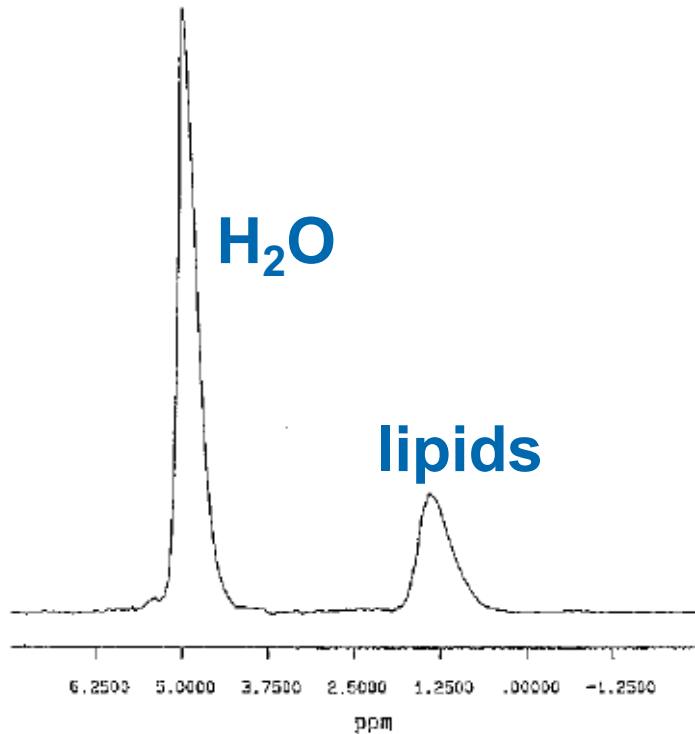


Figure 1. Typical in vivo ^1H spectrum from a steatotic liver (TR = 3 seconds, TE = 24 and 50 msec, four signals acquired, 262 cm^3 volume of interest). No signal filtering before Fourier transformation and no baseline correction were applied.

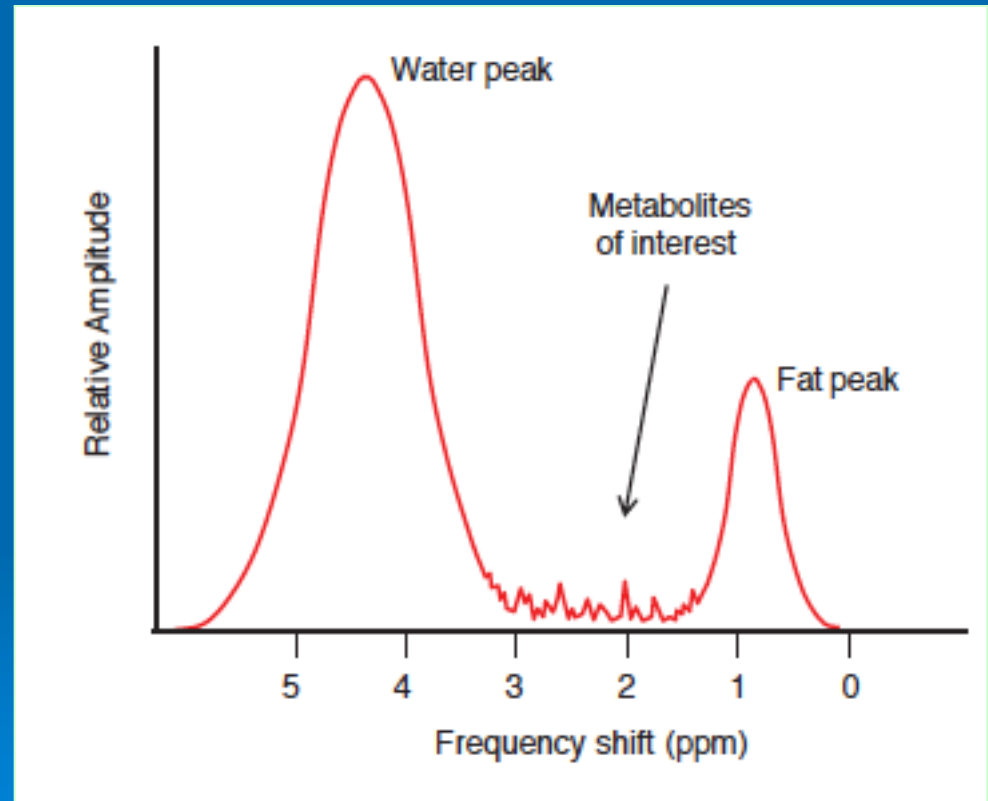

➤ The water signal has to be suppressed

Proton spectroscopy

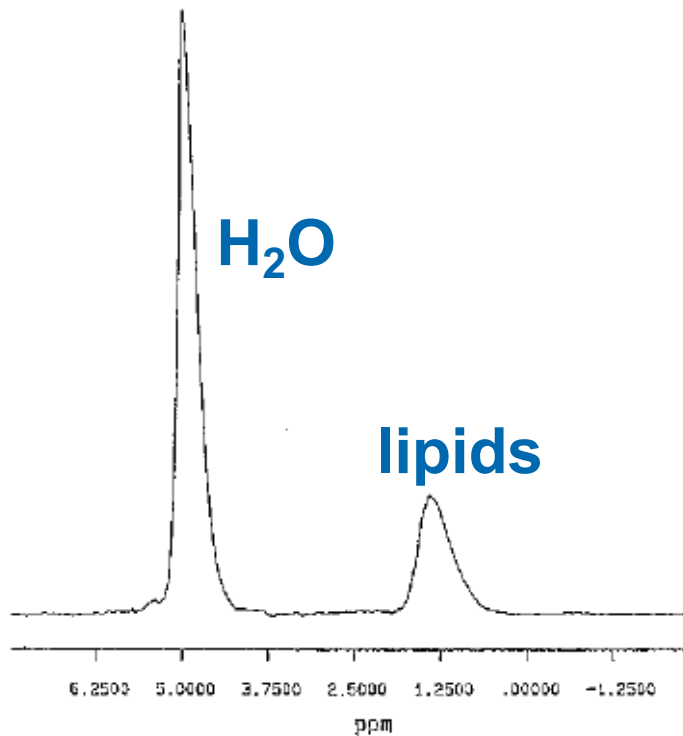


Figure 1. Typical in vivo H-1 spectrum from a steatotic liver (TR = 3 seconds, TE = 24 and 50 msec, four signals acquired, 262 cm³ volume of interest). No signal filtering before Fourier transformation and no baseline correction were applied.


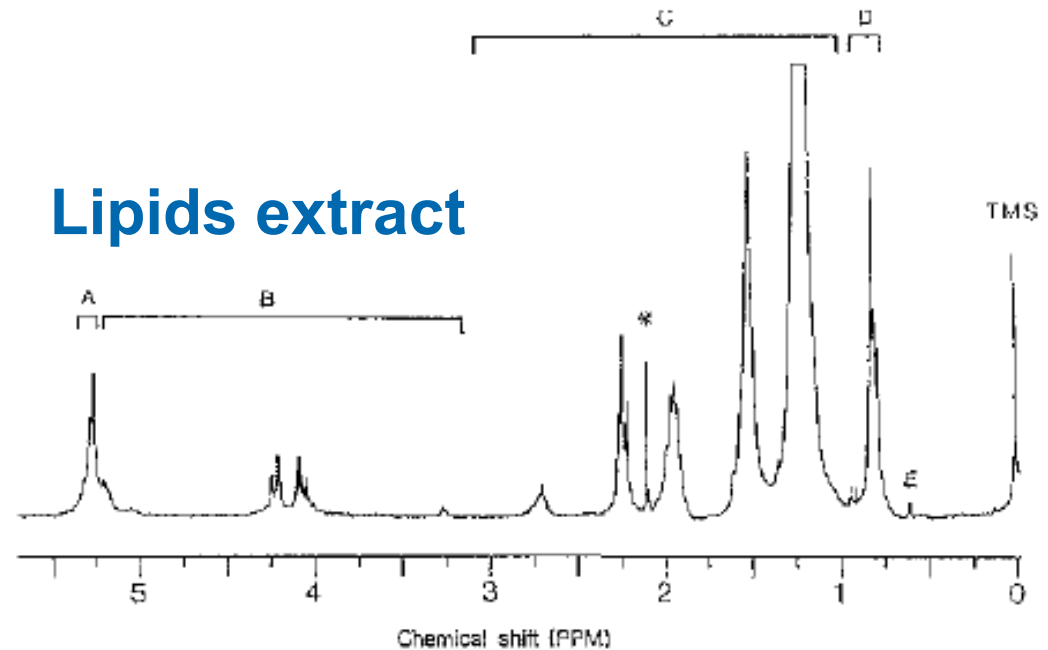


Figure 2. H-1 300-MHz spectrum of lipid extract obtained from a steatotic liver specimen. The major peaks assignable to protons in different positions on lipid molecules are (A) double bonds, (B) protons belonging to di- or triacylated glycerol and to the phosphocholine and phosphoethanolamine components of phospholipids, (C) methylene groups, (D) methyl groups, and (E) methyl signal assigned to carbon-18 of cholesterol. Acetone (*) and tetramethylsilane (TMS) (internal standard) are also shown.

➤ The water signal has to be suppressed

Water suppression

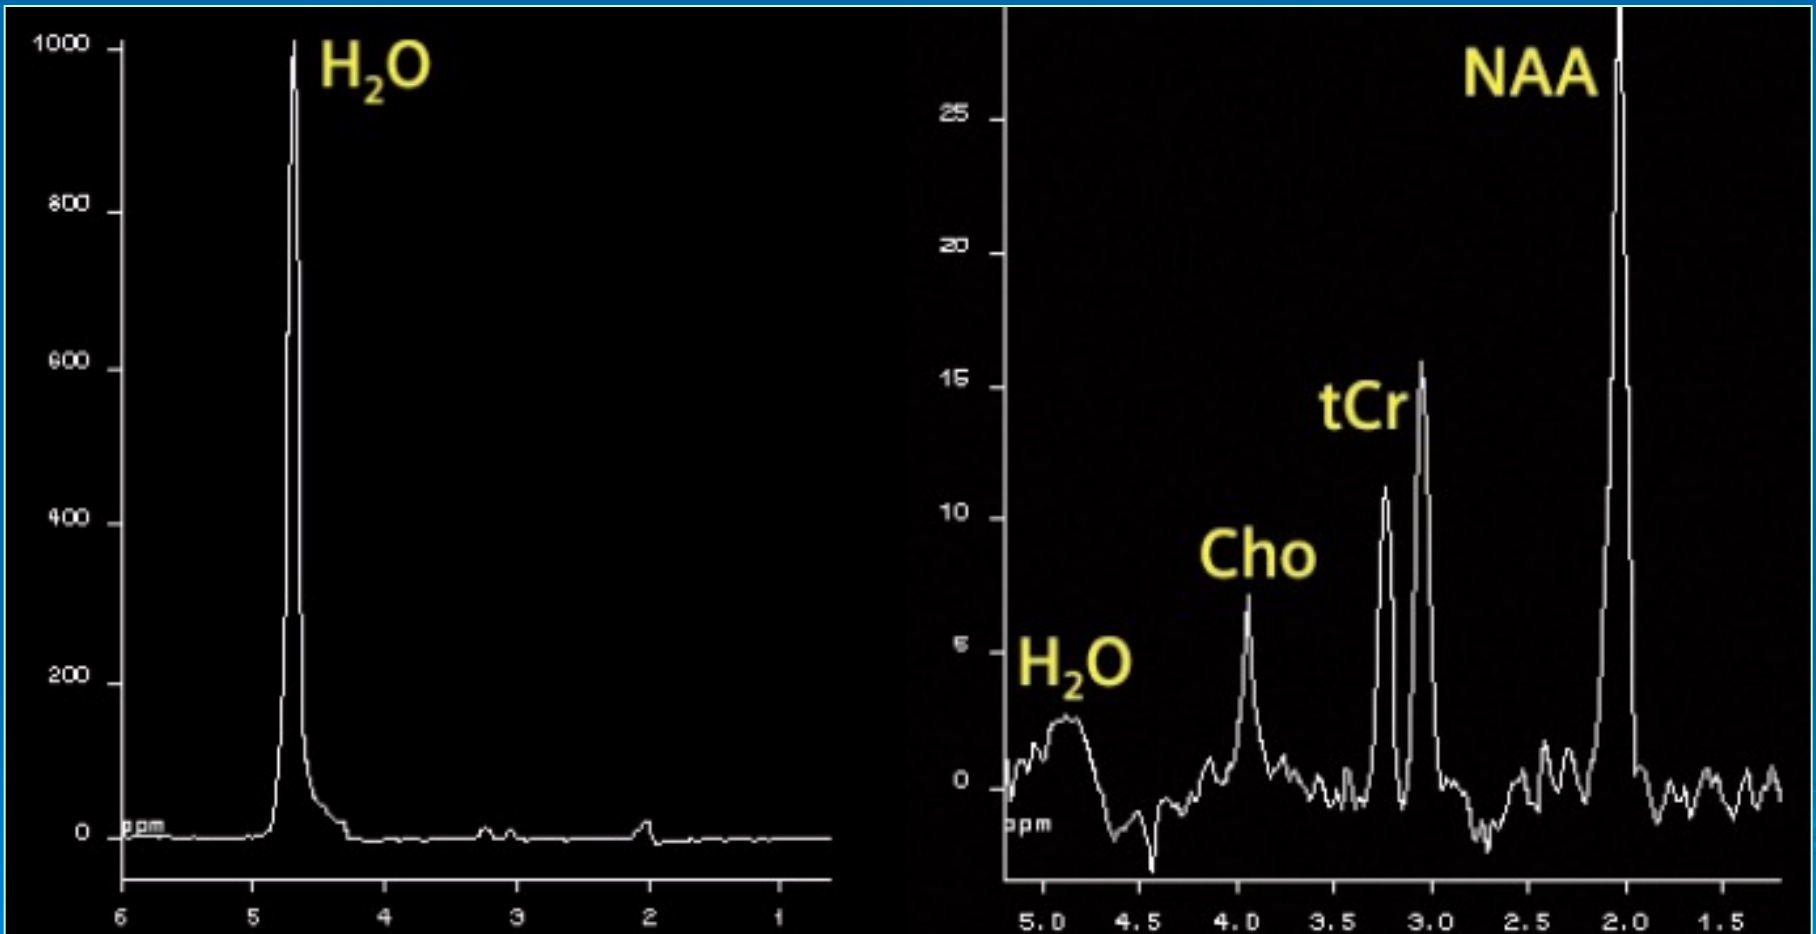

Spectrum without and with water suppression
Different scaling


^1H MRS metabolites

ABBREVIATION	METABOLITE	SHIFT (PPM)	PROPERTIES/SIGNIFICANCE IN THE BRAIN
Cho	Phosphocholine	3.22	Membrane turnover, cell proliferation
Cr	Creatine	3.02 and 3.93	Temporary store for energy-rich phosphates
NAA	<i>N</i> -acetyl-L-aspartate	2.01	Presence of intact glioneuronal structures
Lactate		1.33 (inverted)	Anaerobic glycolysis
Lipids	Free fatty acids	1.2–1.4	Necrosis


Brain spectroscopy

- The ^1H (or ^{31}P) nuclei in different molecules have slightly different resonance frequencies
- Each peak is related to a molecule (metabolite)

In vivo ^1H spectrum

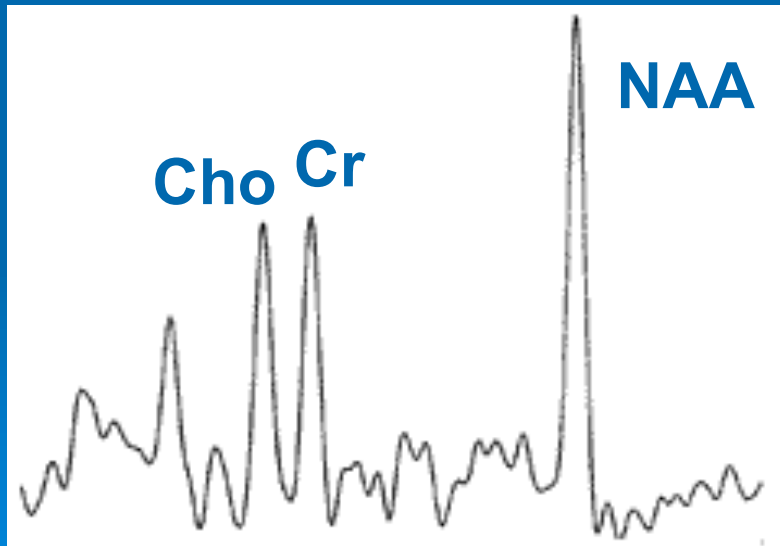


In vivo ^{31}P spectrum

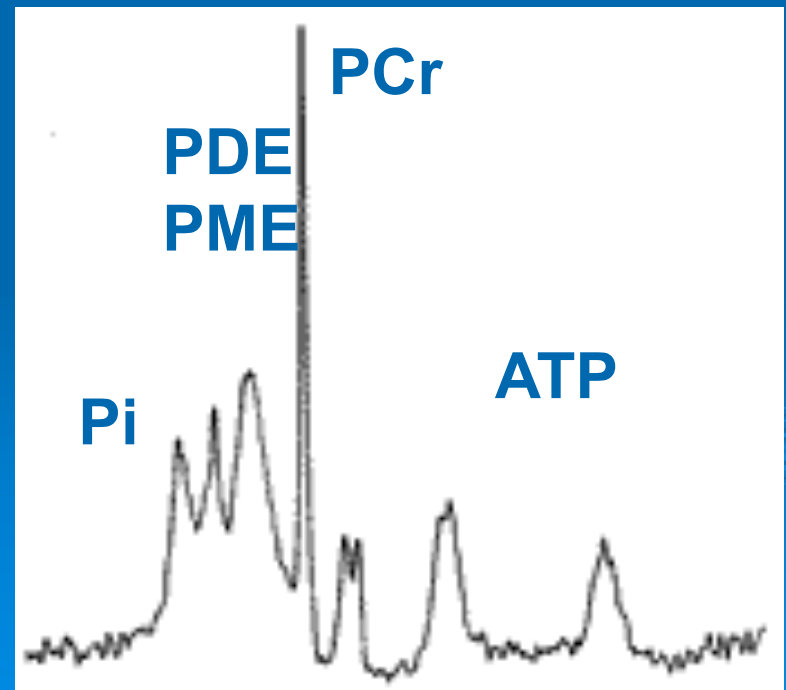


- Occipital cortex


In vivo biochemistry

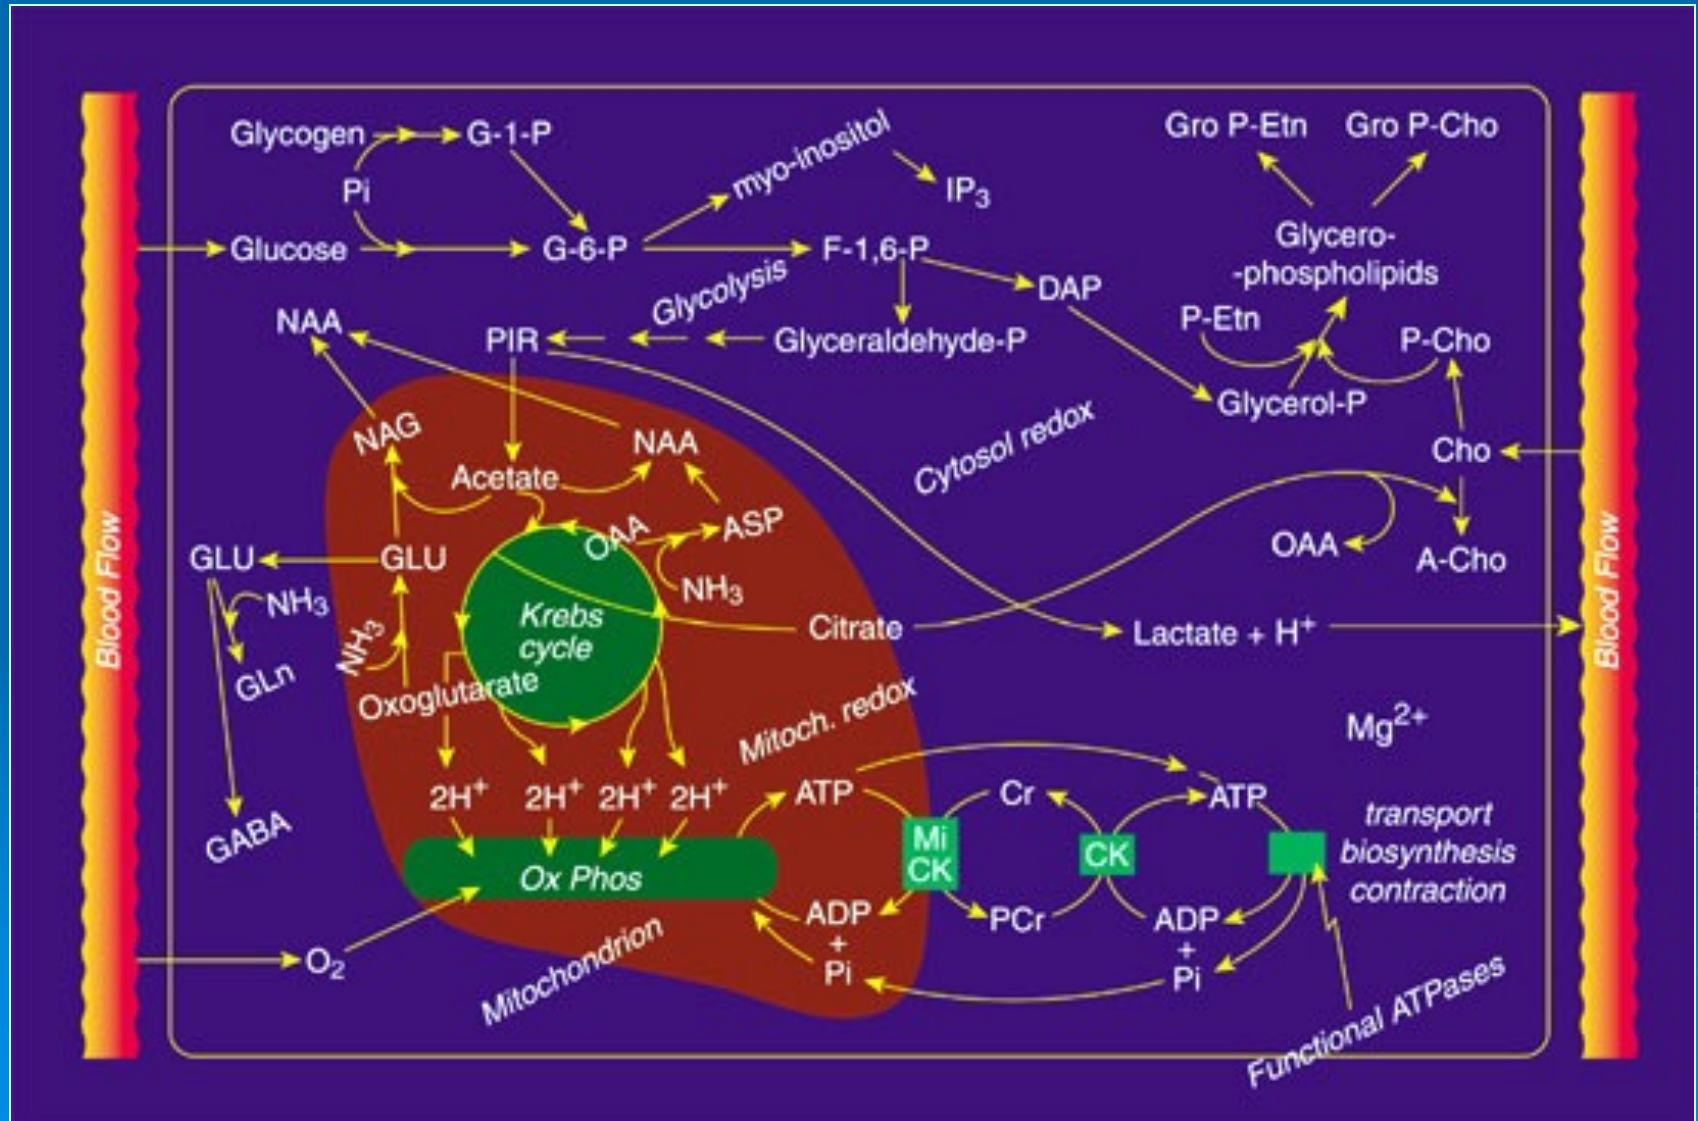


¹H spectroscopy

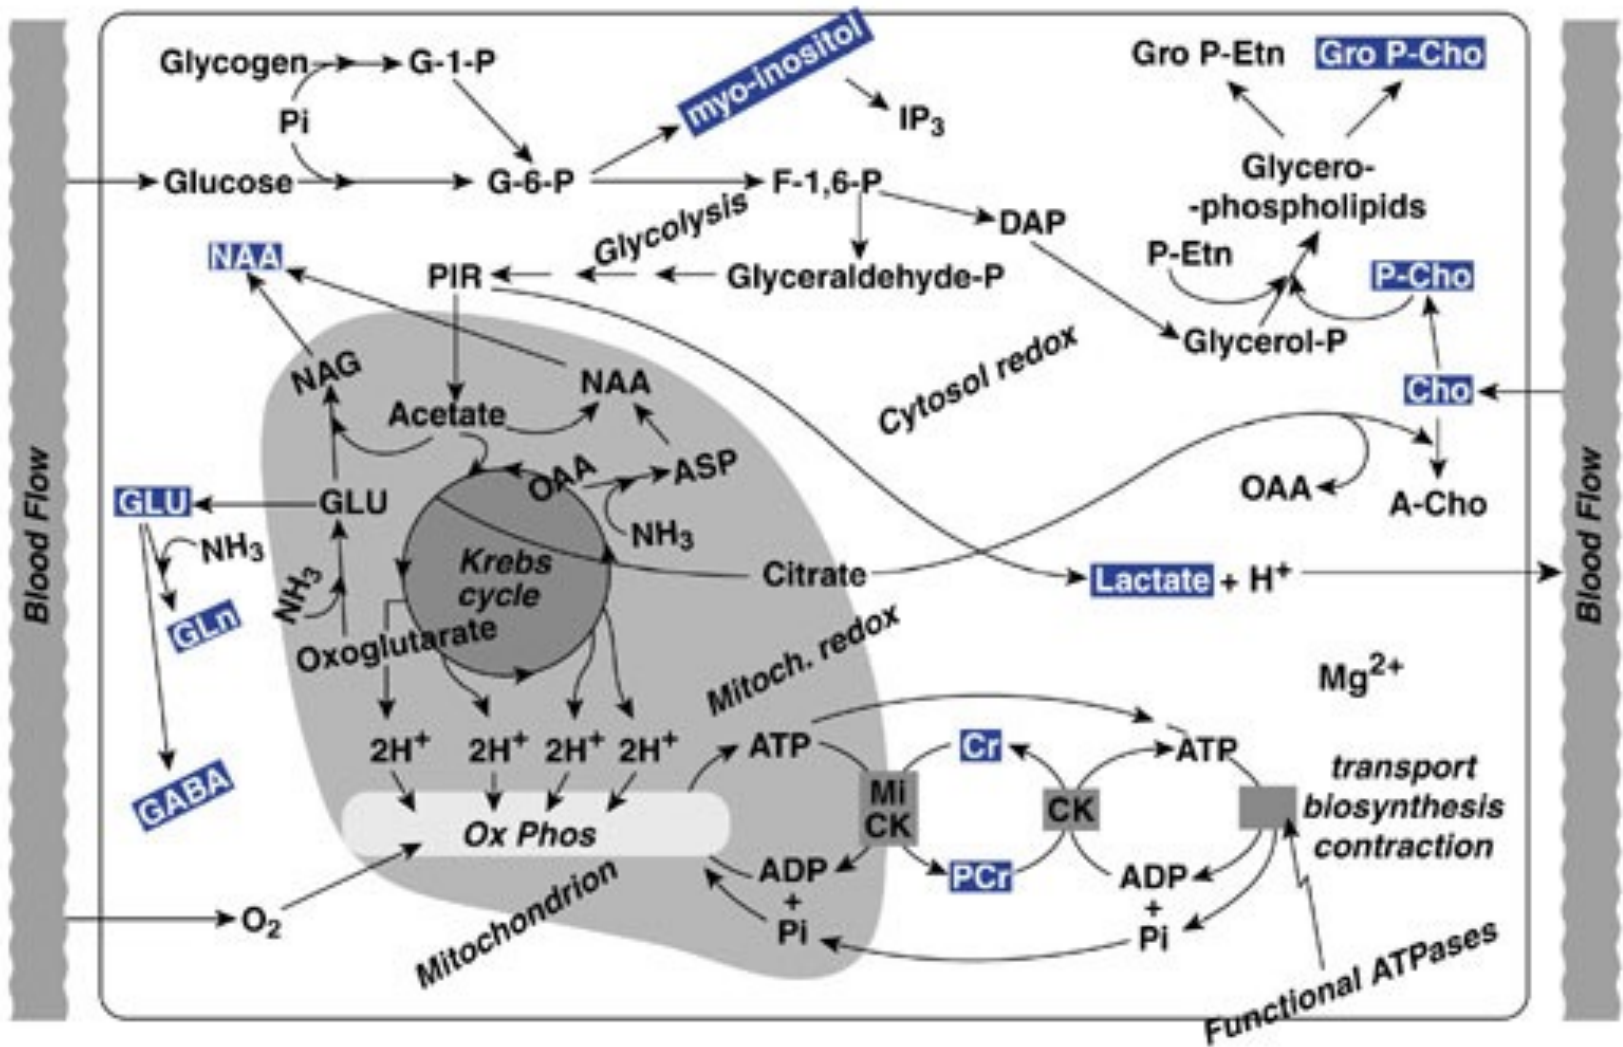

^1H spectroscopy

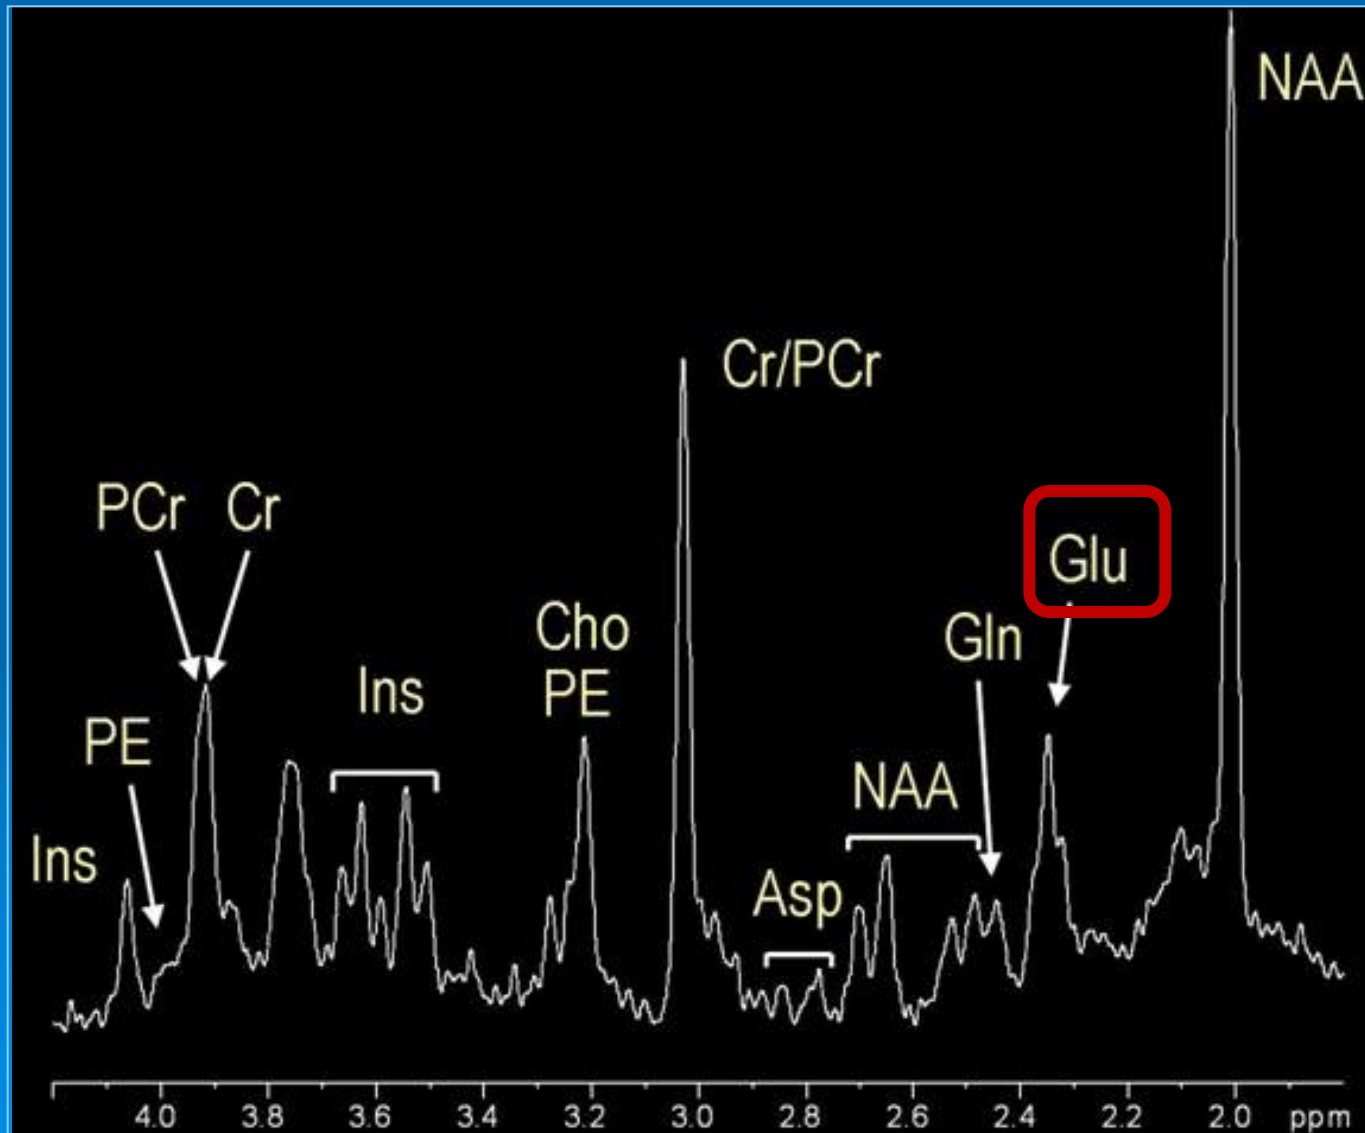


^{31}P spectroscopy

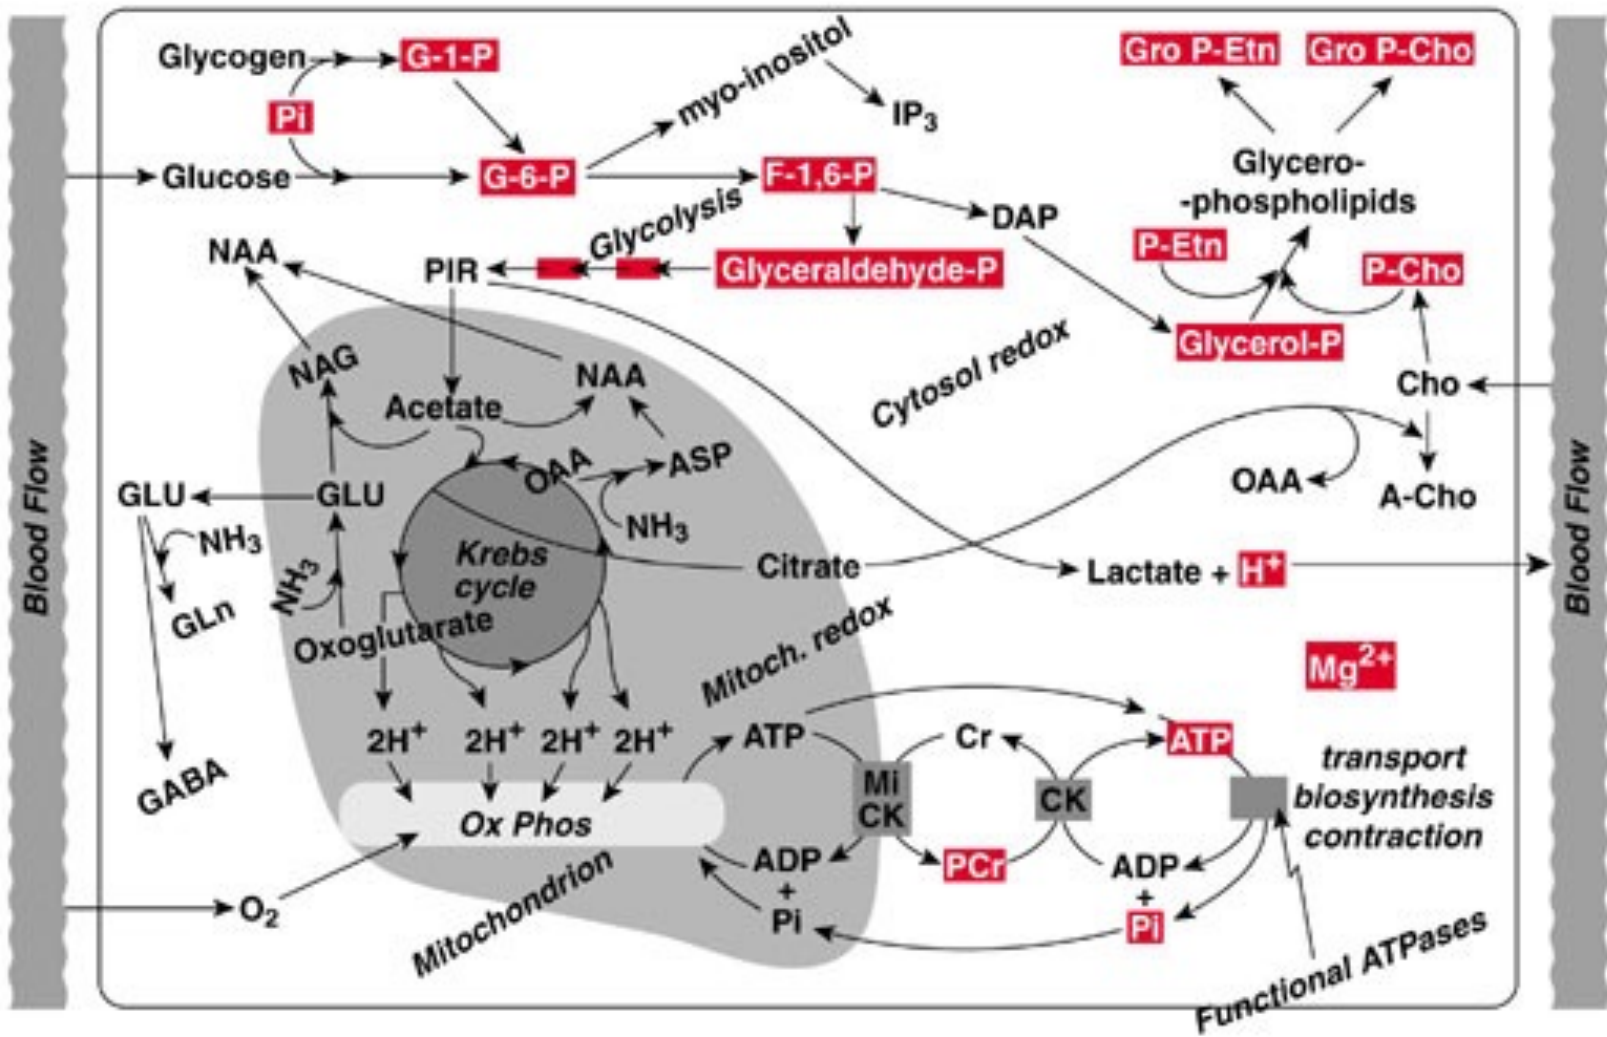

^{31}P MRS

A

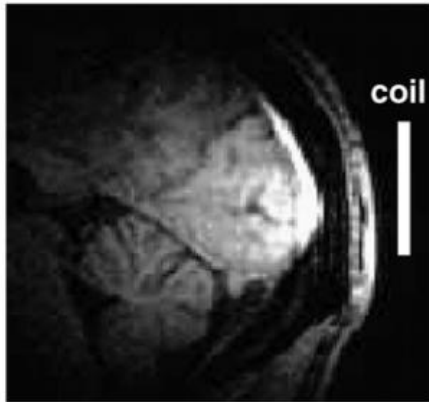

coil

PCr

γ -ATP

α -ATP

β -ATP

B

Pi

C

PE

PC

GPE

GPC

NADP

10

5

0

-5

-10

-15

-20

-25

ppm


In vivo ^{31}P spectra acquired from the human occipital lobe at (B) 4 T and (C) 7 T:

- PE phosphoethanolamine
- PC phosphocholine
- Pi inorganic phosphate
- GPE glycerophosphoethanolamine
- GPC, glycerophosphocholine
- PCr phosphocreatine
- ATP adenosine triphosphate
- NADP nicotinamide adenine dinucleotide phosphate


muscle ^{31}P MRS

- Muscoli gastrocnemi normal subject

rest

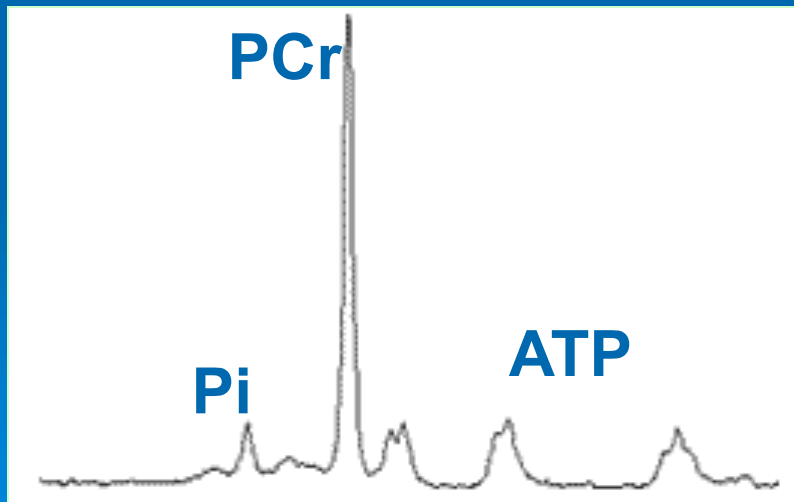


exercise

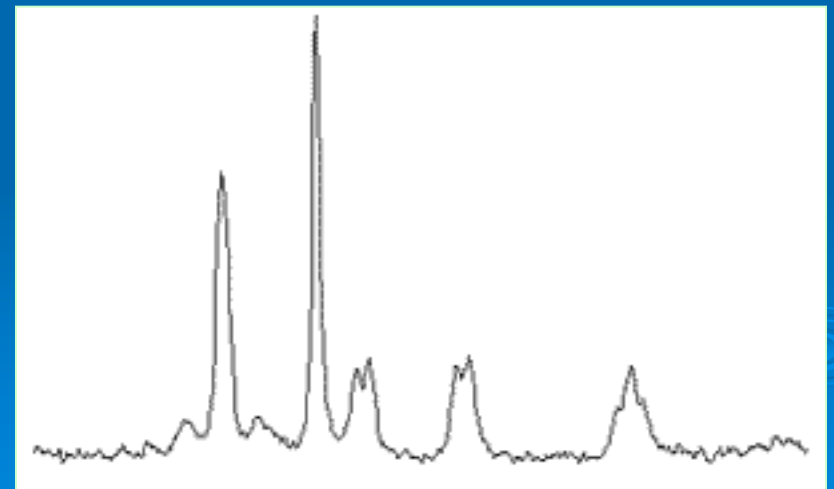


Signal localization

In *in vivo* MRS the signal localization is mandatory

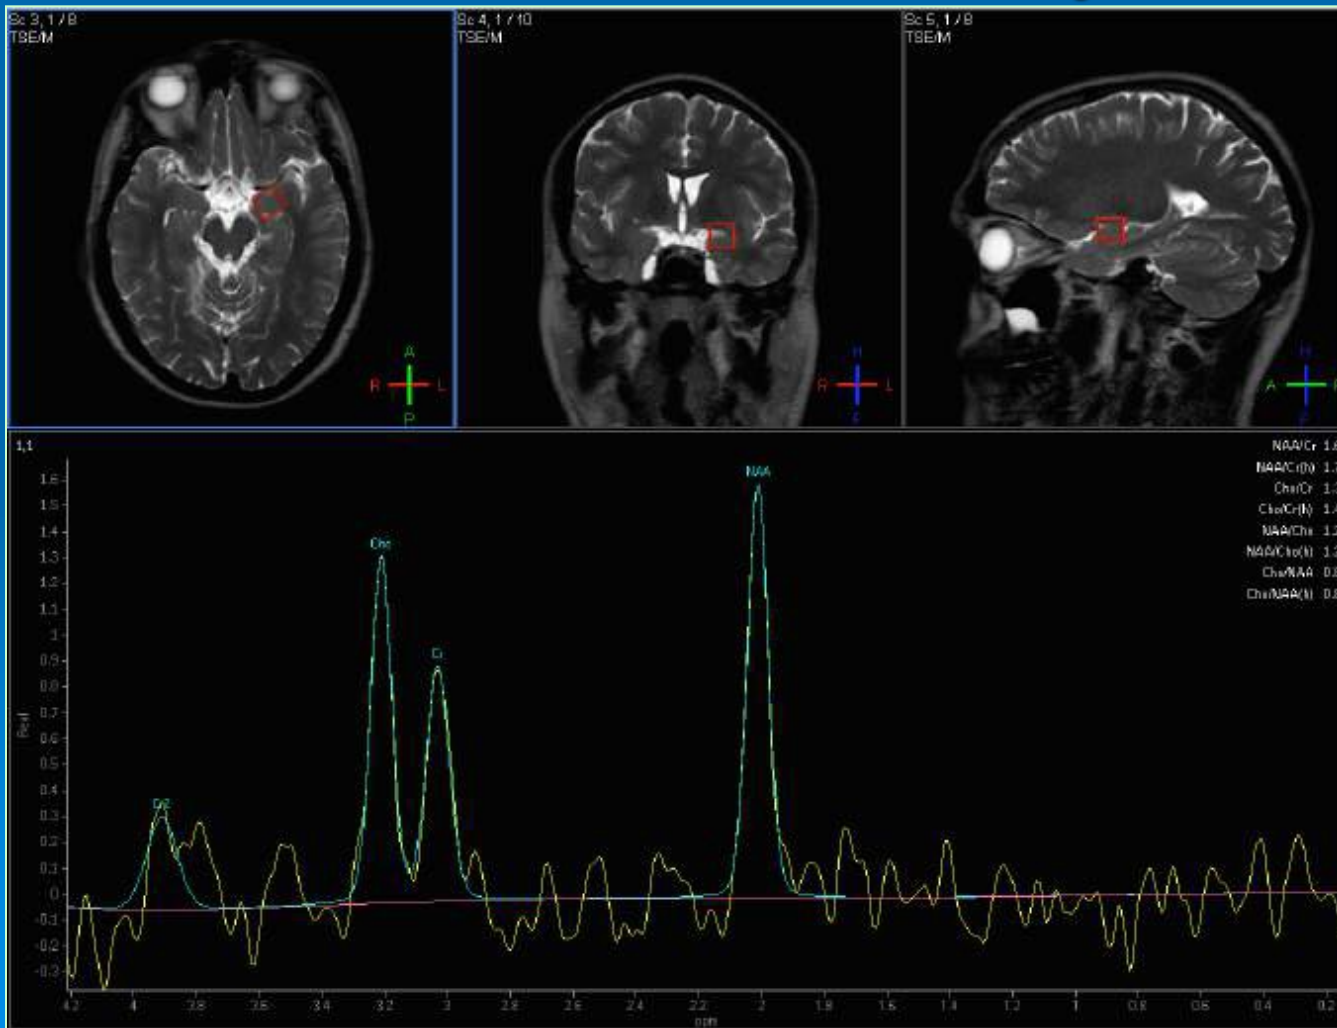



Signal localization

- In in vivo MRS the signal localization is mandatory

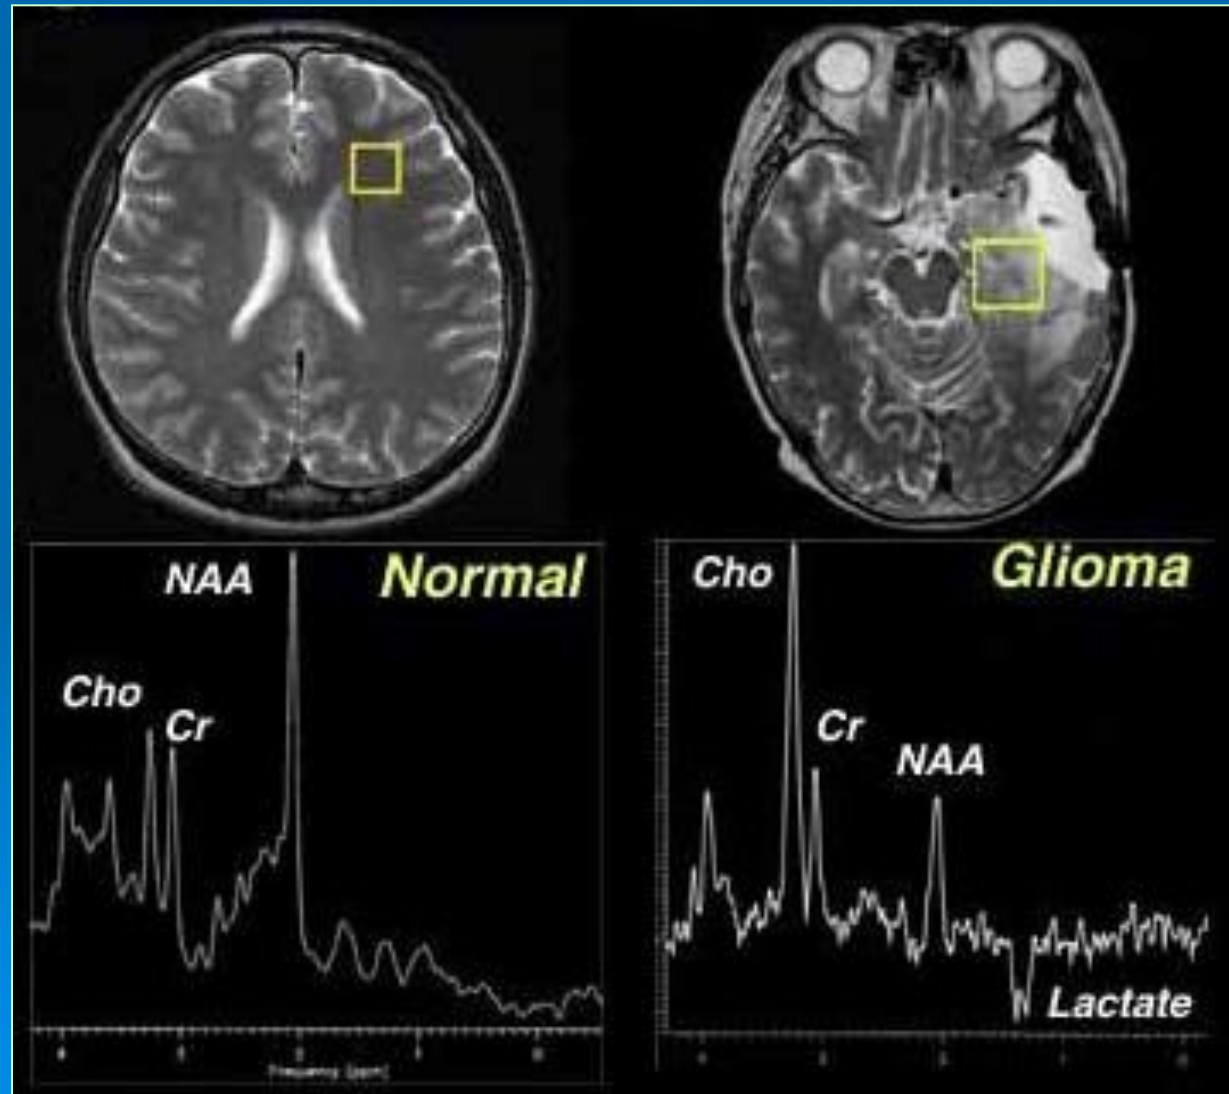


Volume selection

- ✓ The localization of the MRS signal is essential for in vivo application
- ✓ Gradients are used localized spectroscopy
- ✓ The simplest localization technique is the use of the surface coil

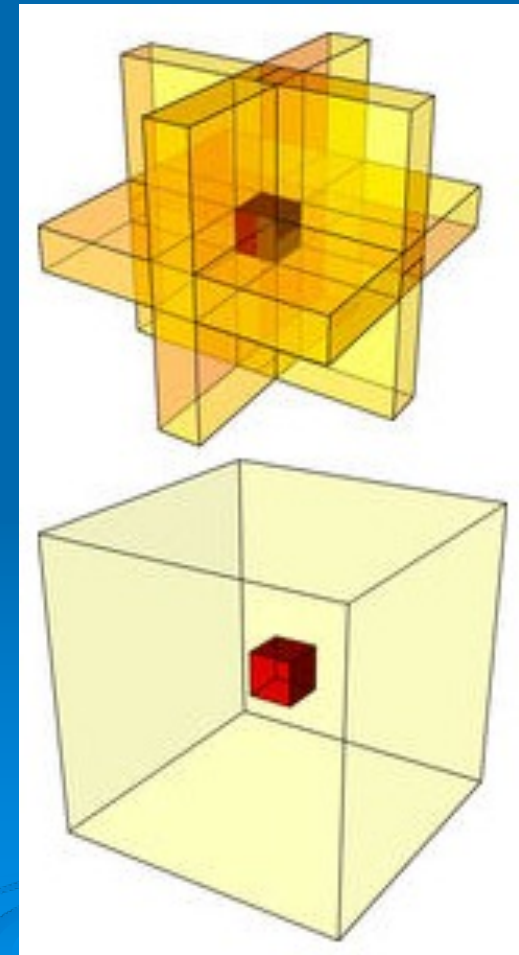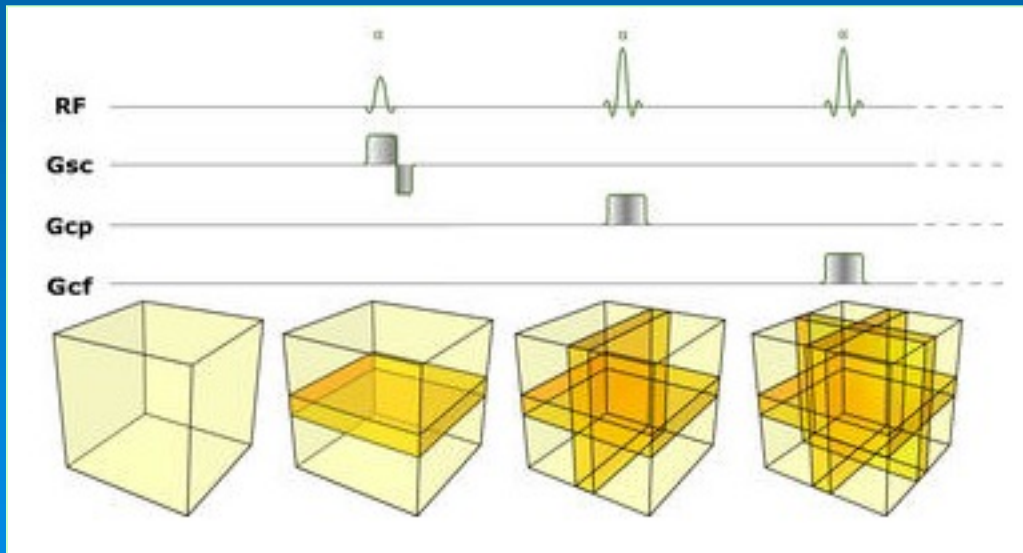



Spectroscopic imaging (Chemical shift imaging CSI)

- ✓ CSI is an acquisition sequence that allows the acquisition of a spectrum per each voxel
- ✓ The acquisition time is large (> 10 minutes)

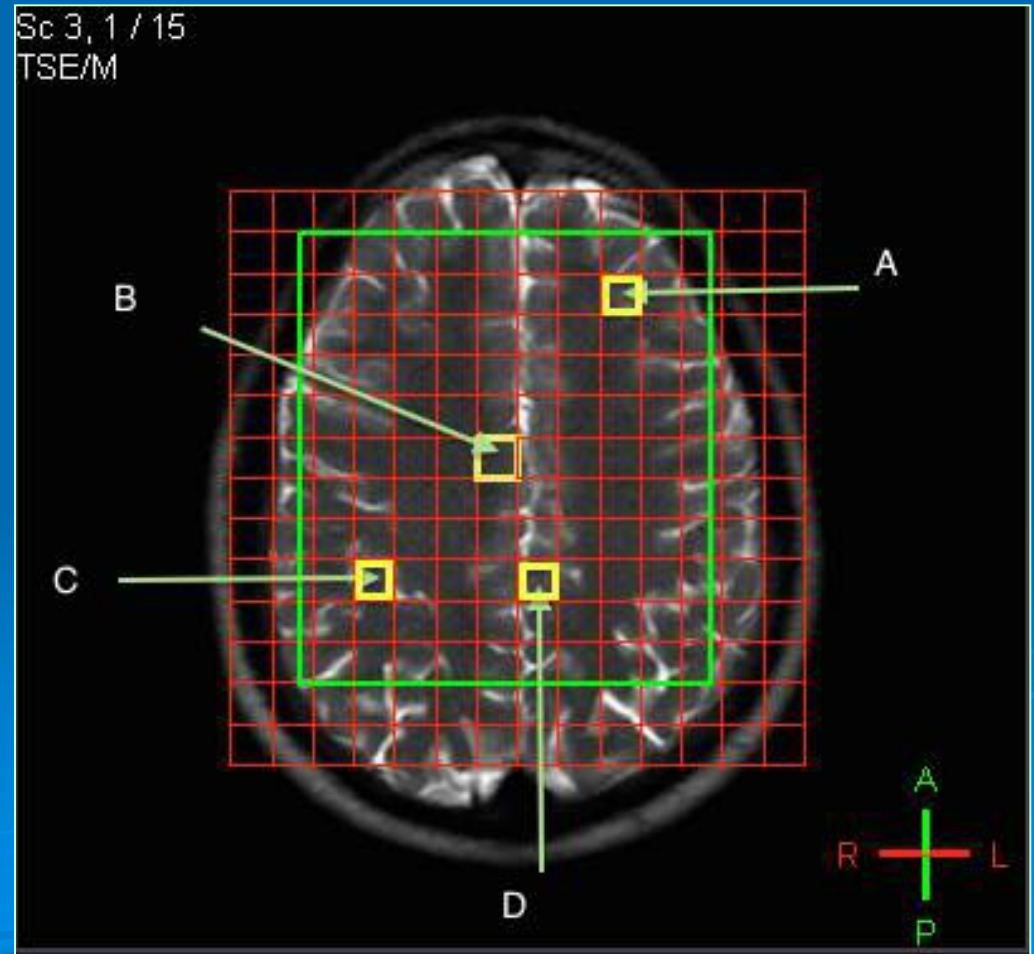


Spectroscopic imaging


- ✓ CSI is an acquisition sequence that allows the acquisition of a spectrum per each voxel
- ✓ The acquisition time is large
 - > 10 minutes

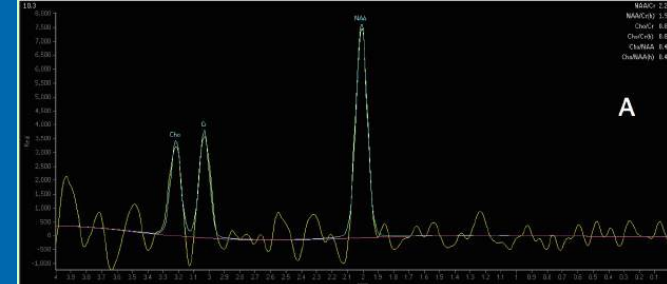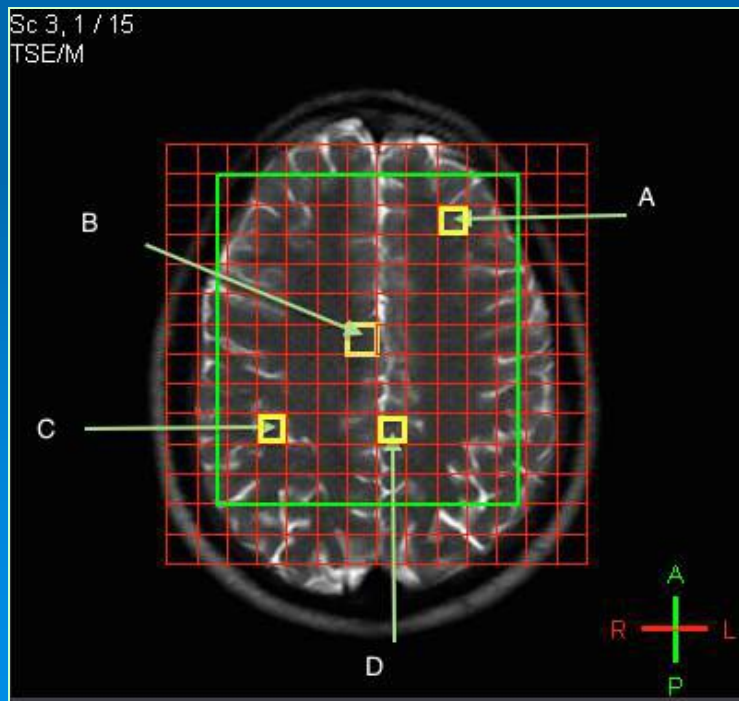


Metab	Position	SNR	Width	Height	FWHM	Area	AreaCr
NAA	2.007	3213	0.884	77266	1.996	7291	3.228
Cr	3.001	1614	0.978	3883	1.993	3258	1.000

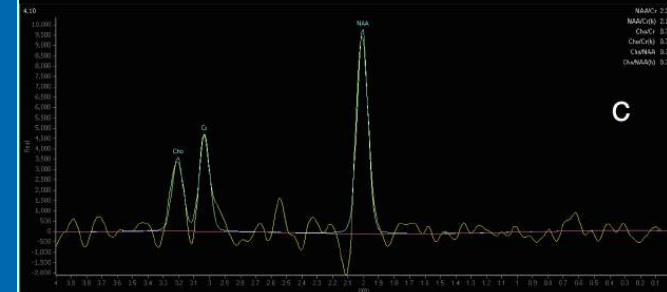

Metab	Position	SNR	Width	Height	FWHM	Area	AreaCr
NAA	2.005	3264	0.882	88869	2.012	8177	2.994
Cr	3.002	1458	0.978	4638	2.008	4129	1.000

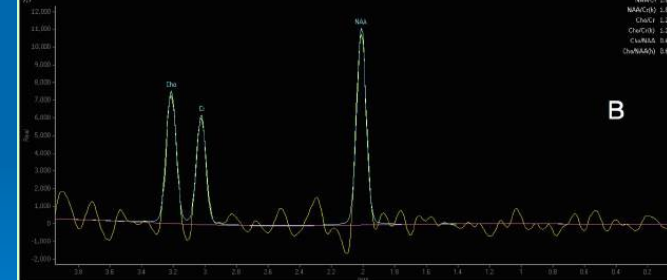


Metab	Position	SNR	Width	Height	FWHM	Area	AreaCr
NAA	2.000	4262	0.867	11577	1.796	8387	1.825
Cr	3.003	2274	0.966	6235	1.999	4919	1.000

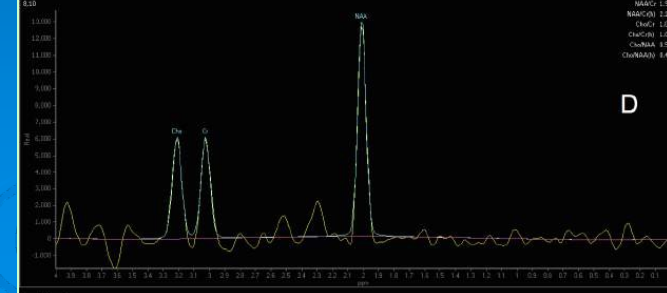

Metab	Position	SNR	Width	Height	FWHM	Area	AreaCr
NAA	2.000	3514	0.862	22923	2.120	8922	1.971
Cr	3.004	713	0.967	6968	1.999	4526	1.000


Spectroscopic imaging (Chemical shift imaging CSI)

- ✓ CSI is an acquisition sequence that allows the acquisition of a spectrum per each voxel
- ✓ The acquisition time is large (> 10 minutes)

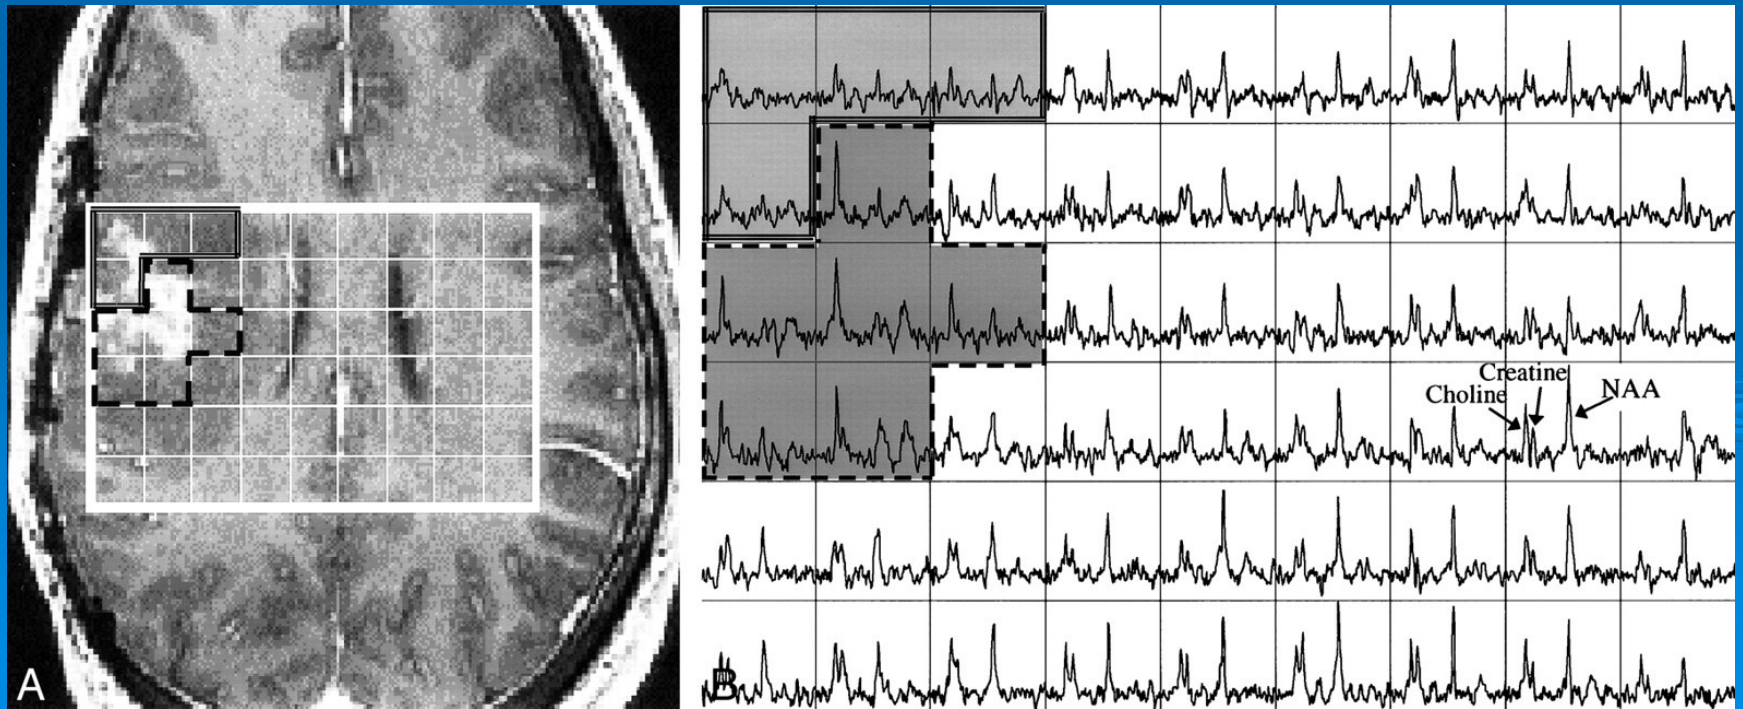



Spectroscopic imaging (Chemical shift imaging CSI)

Magnetic Resonance Spectroscopy

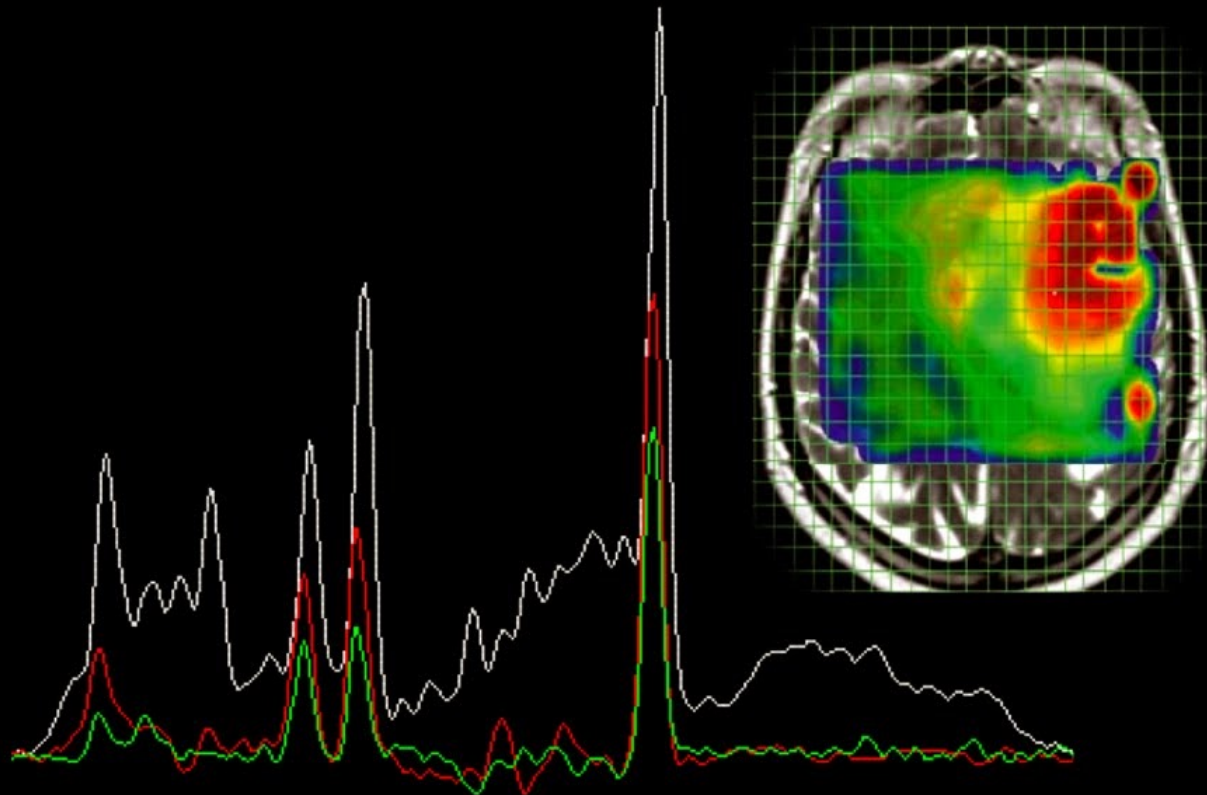



Spectroscopic imaging (Chemical shift imaging CSI)

RadioGraphics 2006; 26:S173-S189

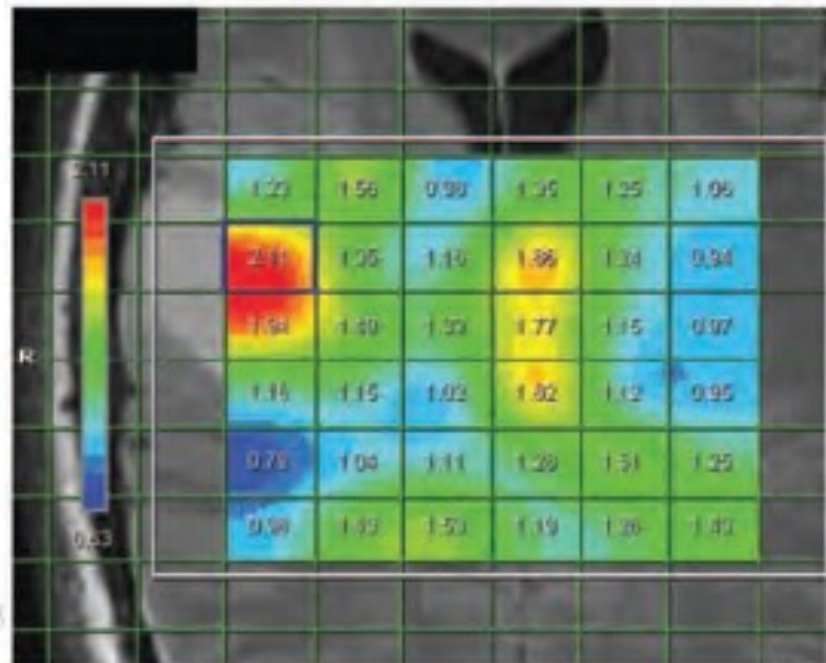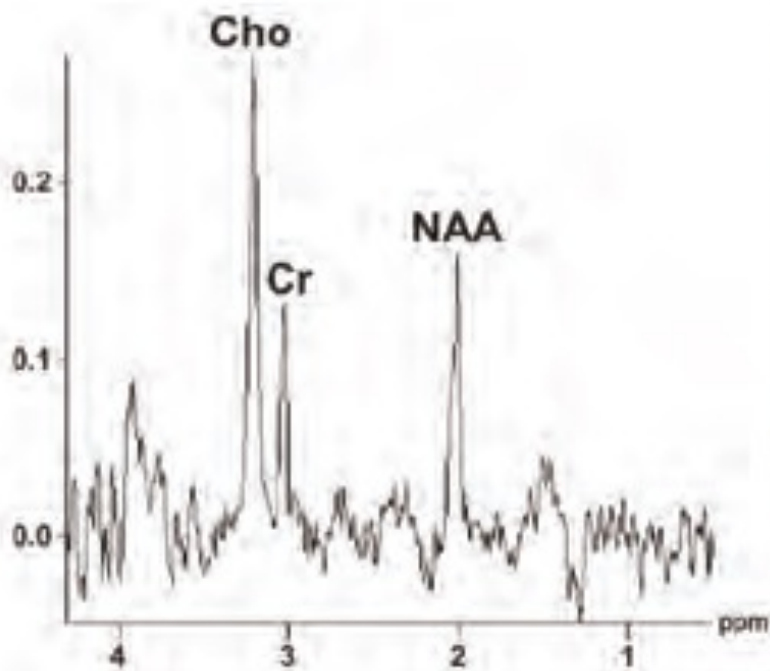

MR Spectrum from anaplastic oligoastrocytoma Choline / Creatine ratio map

Quantitative data analysis

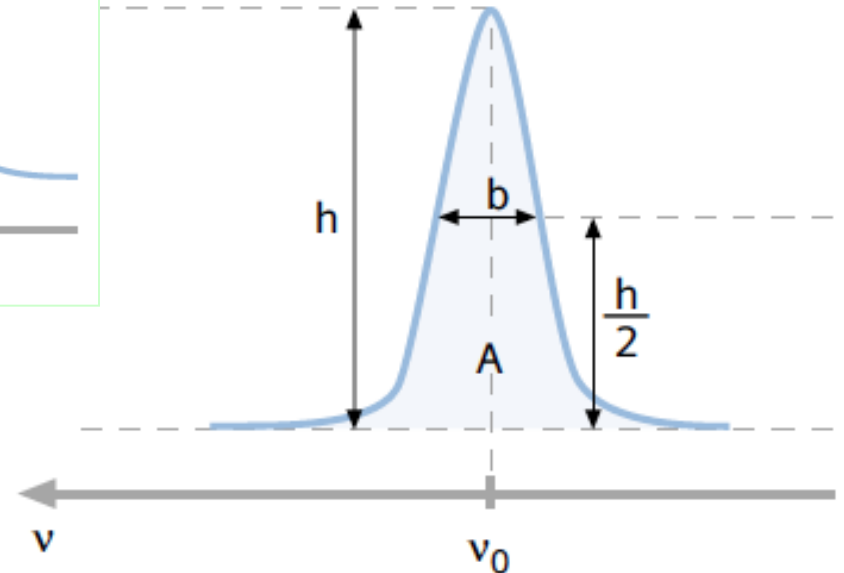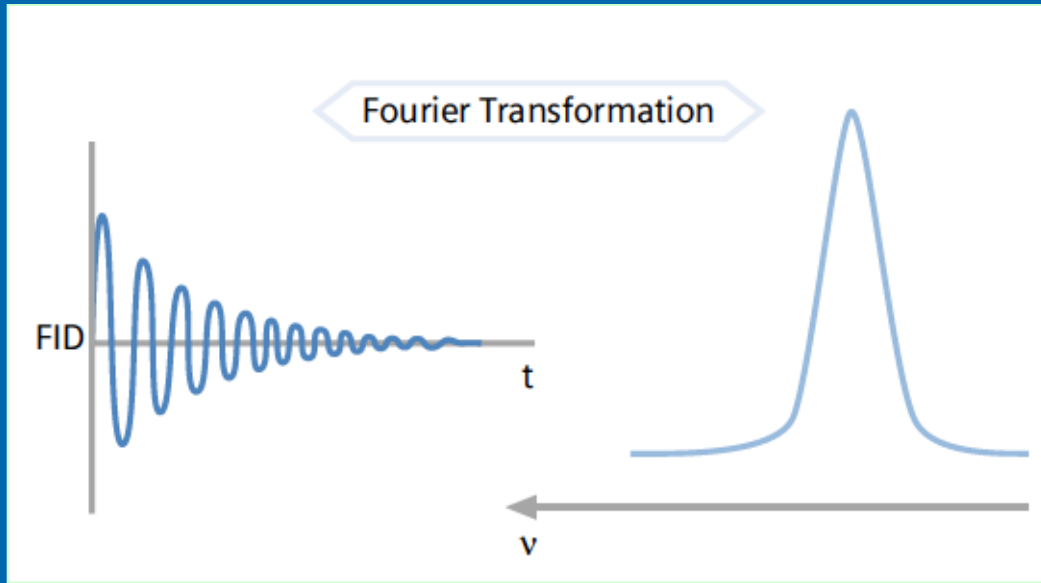

- Resonance frequency: v_0
- Height of peak: h
- Full Width at Half Maximum, FWHM: b
- Integral: A

Applications



Functional Magnetic Resonance Spectroscopy: The “New” MRS for Cognitive Neuroscience and Psychiatry Research

Jeffrey A. Stanley^{1*} and Naftali Raz^{2,3,4}

¹Department of Psychiatry and Behavioral Neurosciences, School of Medicine, Wayne State University, Detroit, MI, United States, ²Department of Psychology, Wayne State University, Detroit, MI, United States, ³Institute of Gerontology, Wayne State University, Detroit, MI, United States, ⁴Center for Lifespan Psychology, Max Planck Institute for Human Development, Berlin, Germany

Preliminary evidence of the ability of ¹H fMRS to detect changes in glutamate during various perceptual, motor, and cognitive tasks.

Applications

Magnetic resonance spectroscopy assessment of brain injury after moderate hypothermia in neonatal encephalopathy:

a prospective multicentre cohort study

Peter J Lally et al for the MARBLE consortium

Lancet Neurol 2019; 18: 35–45

Summary

Thalamic proton MRS measures acquired soon after birth in neonatal encephalopathy had the highest accuracy to predict neurodevelopment 2 years later.

Applications

**Magnetic resonance spectroscopy assessment of brain injury after moderate hypothermia in neonatal encephalopathy:
a prospective multicentre cohort study**

Lancet Neurol 2019; 18: 35–45

Methods

- ✓ **3.0 Tesla scanner**
- ✓ **single $15 \times 15 \times 15 \text{ mm}^3$ voxel centred on the left thalamus**
- ✓ **^1H MRS metabolite peak area ratios (7 min)**
- ✓ **^1H MRS metabolite absolute concentrations (25 min)**
- ✓ **diffusion weighted MRI (DW MRI; 7 min)**