

Corso di Biotecnologie applicate
A.A. 2024-2025



Stefano Ceschia

Alifax Srl (Sede di Nimis, Udine)

Trieste, 01st April 2025



UNIVERSITÀ
DEGLI STUDI
DI TRIESTE

1. *General introduction about Alifax, Research and Design activities*
2. *Main areas of interest in Alifax*
 - a) *ESR (scope of the test, biological mechanisms, clinical importance)*
 - b) *Microbiology (Antimicrobial Stewardship, MDROs, Clinical microbiology workflow)*
 - c) *Introduction of new products in the market*
3. *Design process (Project Vision, Stakeholder needs, Usability, Safety, Performance)*
4. *From Design to Manufacturing and Sells: Process Validation, Safety, Registrations*

1. *General introduction about Alifax, Research and Design activities*
2. *Main areas of interest in Alifax*
 - a) *ESR (scope of the test, biological mechanisms, clinical importance)*
 - b) *Microbiology (Antimicrobial Stewardship, MDROs, Clinical microbiology workflow)*
 - c) *Introduction of new products in the market*
3. *Design process (Project Vision, Stakeholder needs, Usability, Safety, Performance)*
4. *From Design to Manufacturing and Sells: Process Validation, Safety, Registrations*

LEADER ITALIANO DELL'IVD

- Alifax opera nella progettazione, produzione e commercializzazione di dispositivi IVD per la diagnostica di laboratorio clinico.
- Distribuisce in Italia prodotti IVD di terzi come importatore e distributore
- Commercializza in Italia e nel mondo i prodotti a proprio marchio






ALIFAX DESIGN AND MANUFACTURING SITE

INSIDE INNOVATION


Alifax has a large facility in Nimis (UD) dedicated to the reasearch, development, design and production of IVD products and service

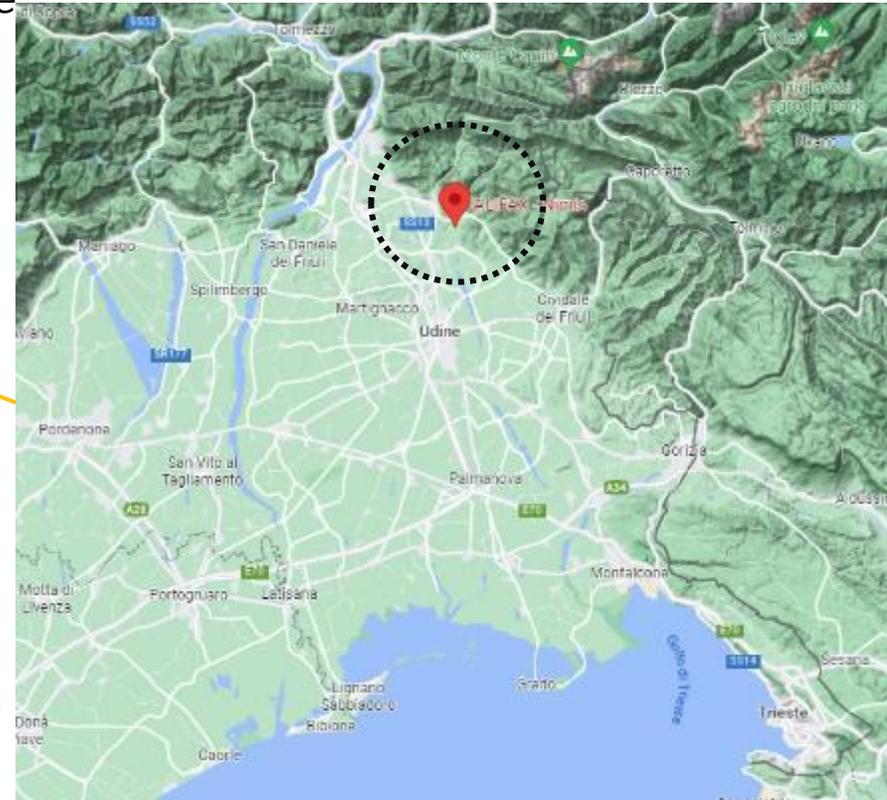




- Approximately 100 persons involved in:
 - R&D;
 - Design;
 - Manufacturing;
 - Quality Assurance & Regulatory affairs (QARA);
 - Administration and logistics



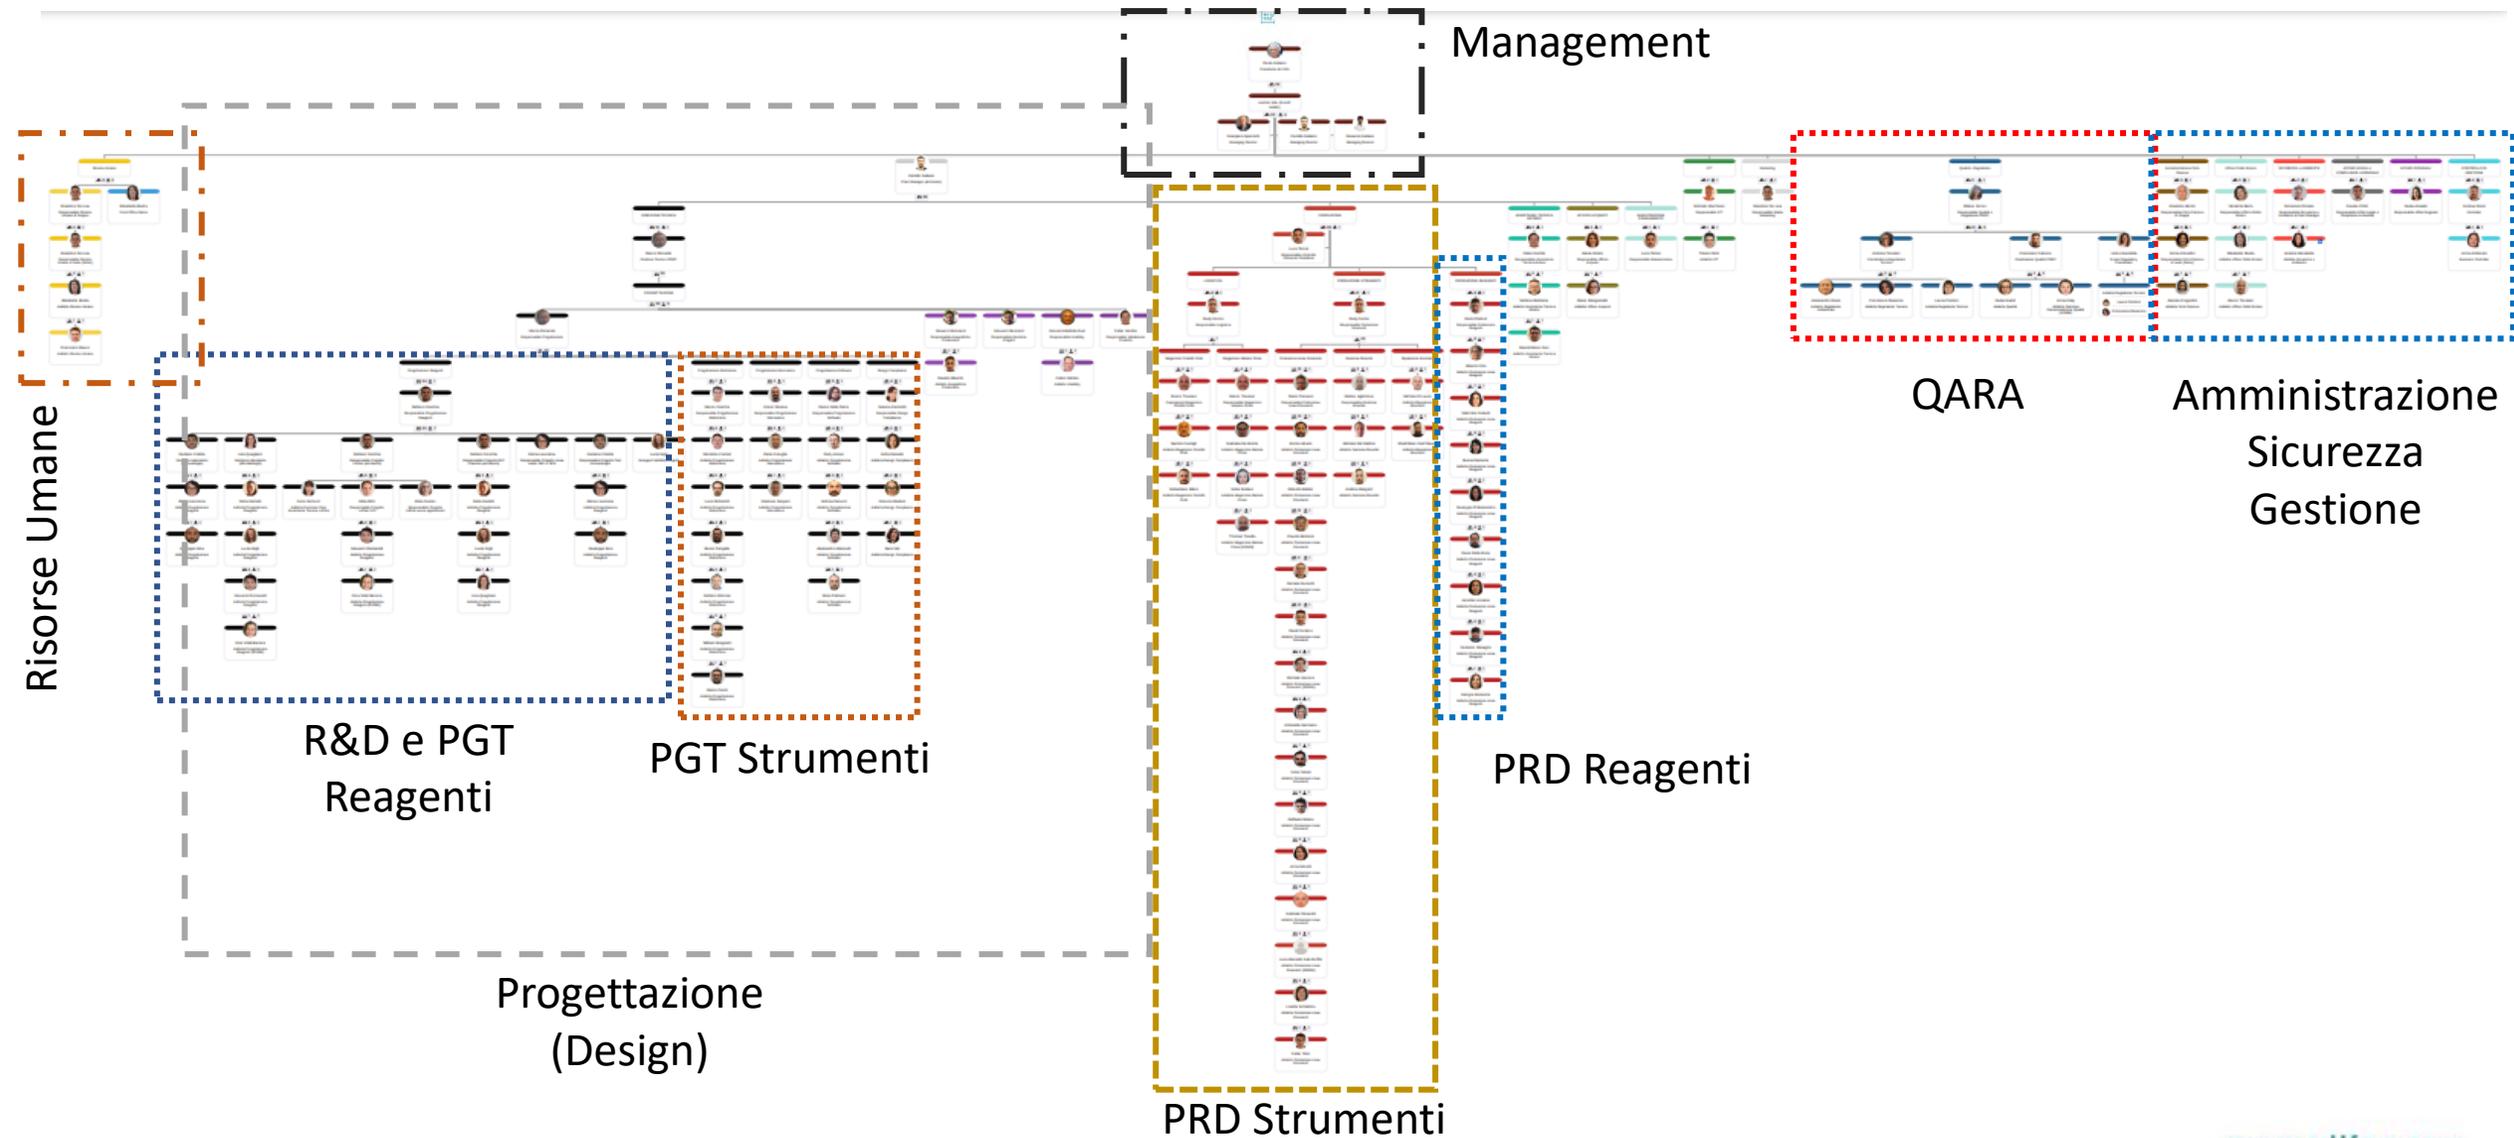

PROGETTAZIONE REAGENTI

- **Professionalita’:**
 - *Biologi;*
 - *Chimici;*
 - *Biotecnologi;*
 - *Tecnici di laboratorio;*
- **Grado di formazione:**
 - *Laurea magistrale;*
 - *PhD*
 - *Post-Doc*

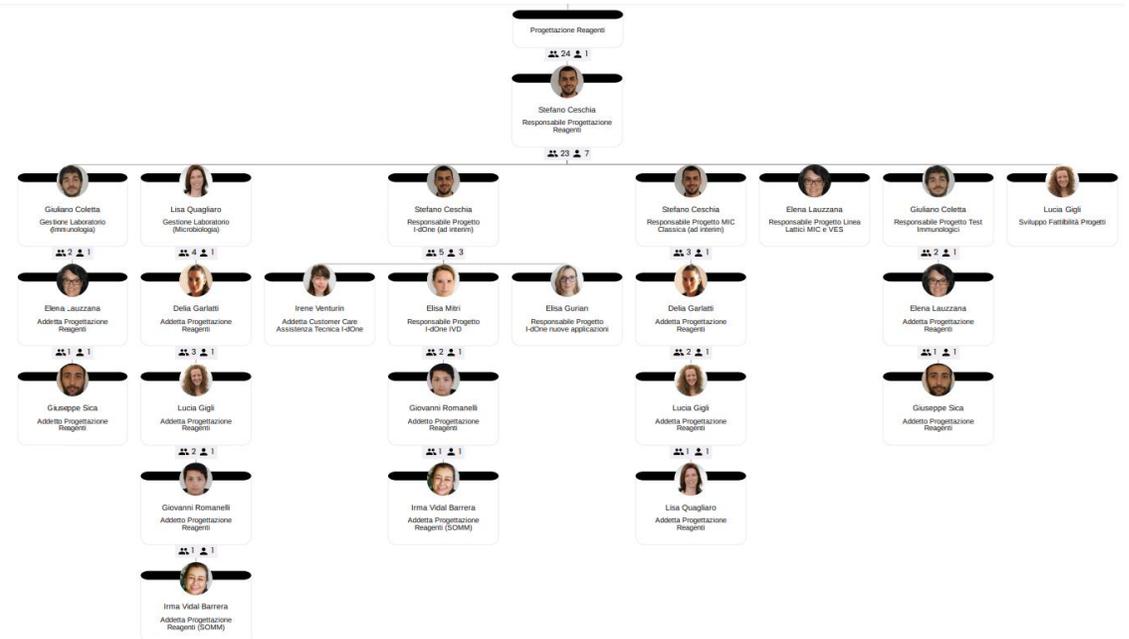

L'UFFICIO RICERCA E SVILUPPO SEDE DI NIMIS

- **Scopo dell'ufficio:**
 - sviluppo di nuovi test sugli strumenti a marchio Alifax;
 - ricerca e testing di nuove tecnologie applicabili all'ambito clinico diagnostico;
 - sviluppo di nuovi dispositivi tramite progetti di prototipizzazione ed industrializzazione.
- **Composizione:**
 - Attualmente impiegate 13 persone di diversa estrazione formativa
- **Background:**
 - 4 risorse con titolo PhD in ambito chimica / biofisica
 - 9 laureati in ambito Biologia, Biotecnologie, Chimica industriale





Progettazione Elettronica



Progettazione Meccanica



Produzione reagenti



Progettazione Software



Validazioni ospedaliere



Utilizzatore finale



Qualità e regolatorio



Progettazione Elettronica




Progettazione Meccanica



Produzione reagenti



Progettazione Software

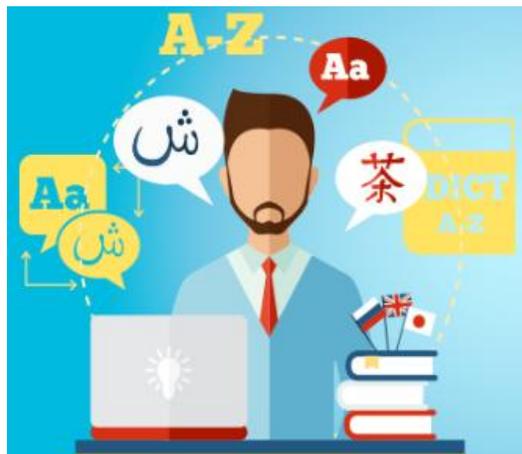

Validazioni ospedaliere



Utilizzatore finale



Qualità e regolatorio

1. *General introduction about Alifax R&D and Design*
2. *Main areas of interest in Alifax*
 - a) *ESR (scope of the test, biological mechanisms, clinical importance)*
 - b) *Microbiology (Antimicrobial Stewardship, MDROs, Clinical microbiology workflow)*
 - c) *Introduction of new products in the market*
3. *Design process (Project Vision, Stakeholder needs, Usability, Safety, Performance)*
4. *From Design to Manufacturing and Sells: Process Validation, Safety, Registrations*



ALIFAX'S PRODUCT LINES

- ESR
- MICROBIOLOGY
- IMMUNOLOGY






ALIFAX'S PRODUCT LINES

- ESR
- MICROBIOLOGY
- IMMUNOLOGY



Exploring the Multifaceted Role of ESR

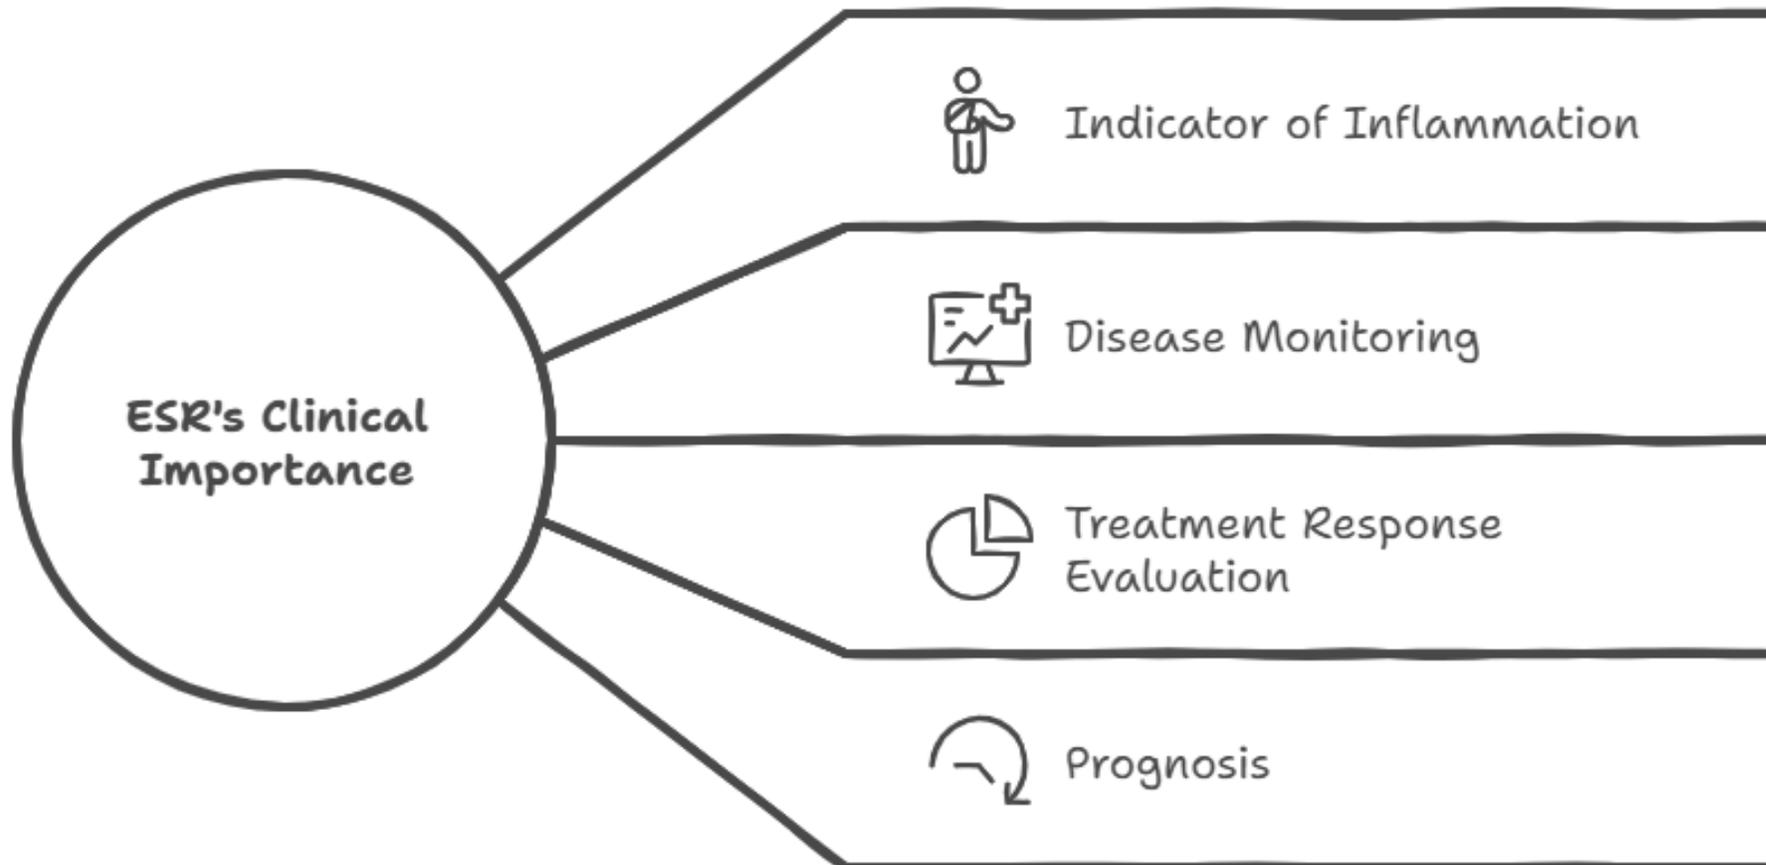

Made with  Napkin

A Bit of History

- Even the ancient **Greeks and Romans** noticed a different blood sedimentation in various medical disorders
- During the **Middle Ages** and the **Renaissance** physicians describe in specific diseases of blood clots covered with whitish liquid called "crusta inflammatoria"
- In **1772 William Hewson** in **1832** and **Herman Nasse** observe that the sedimentation in blood samples without fibrinogen is much slower than the whole blood samples
- In **1894, Edmund Biernacki** (1866-1912), a Polish physician, first noted the increased sedimentation rate of blood from ill individuals and realized that this increase was due to the **presence of fibrinogen** in the individual's blood sample.



Edmund Biernacki
(1866-1912)

A Bit of History

- In **1918**, **Robin Fahraeus** (1888-1968) furthered Biernacki's work. His initial motivation to study the ESR of blood was as a **pregnancy test**, but his interest expanded to the study of the ESR test in his patients.
- In **1921**, **Alf Westergren** (1881-1968) refined the technique of performing the ESR test and reported its usefulness in determining the prognosis of patients with **tuberculosis**.
- In **1935**, **Maxwell M. Wintrobe** (1901-1986) published a variation of the ESR methodology and, at one time, this method was in wide use.










National Museum of the History of
Science and Medicine
(The Netherlands)
Erythrocyte sedimentation rate
equipment stand (CEMI 1920)

ESR

THE STANDARD METHOD


ESR

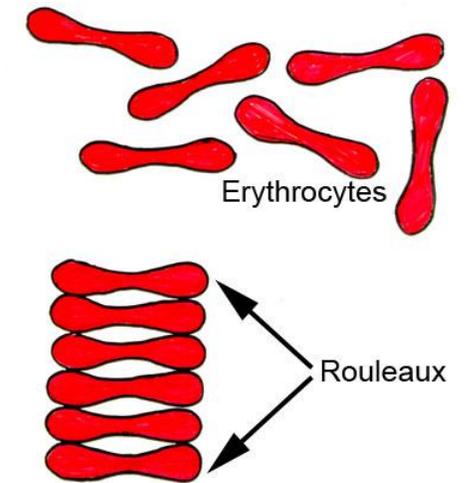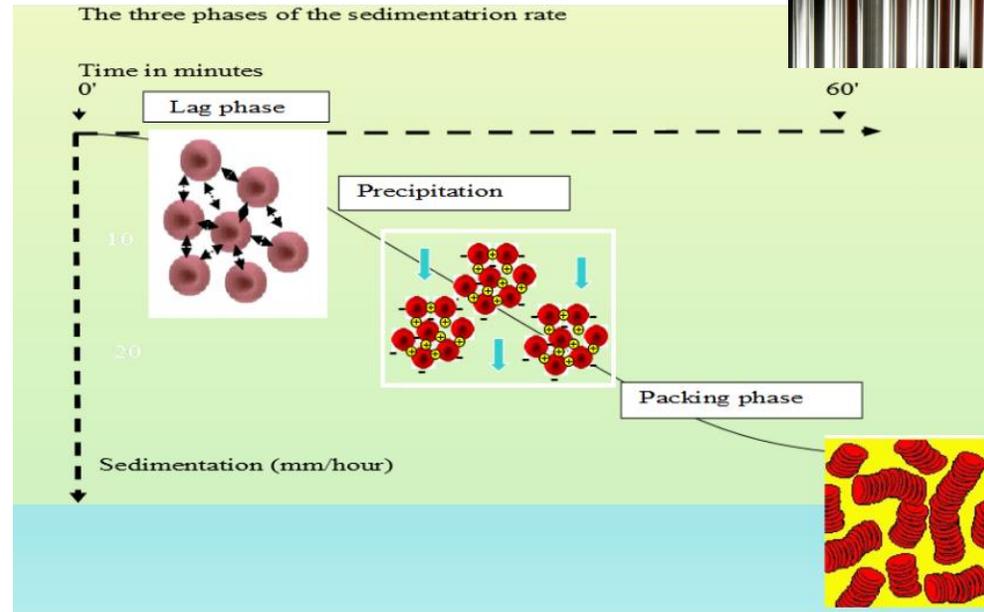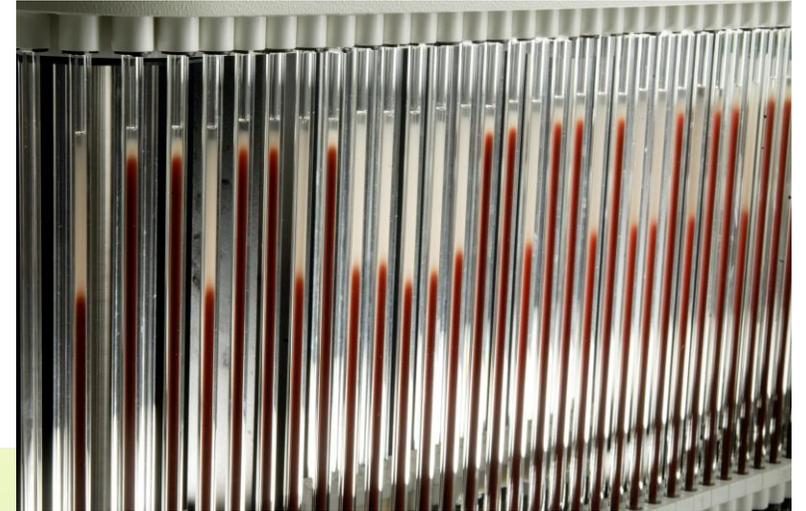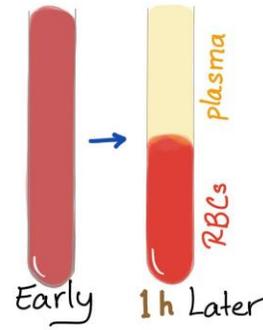

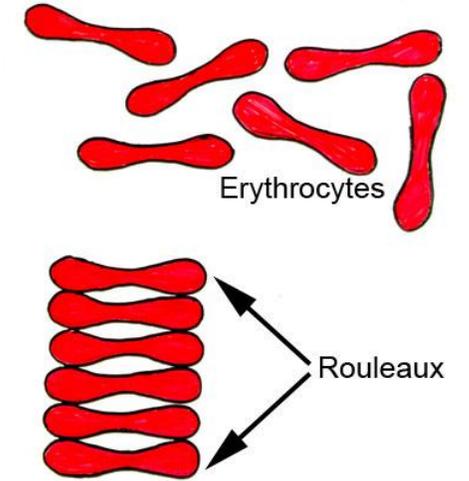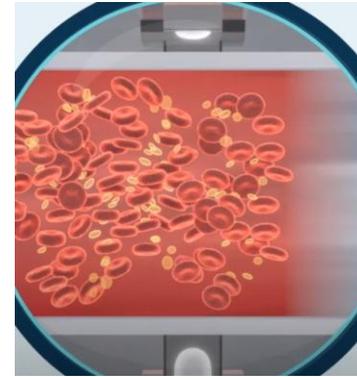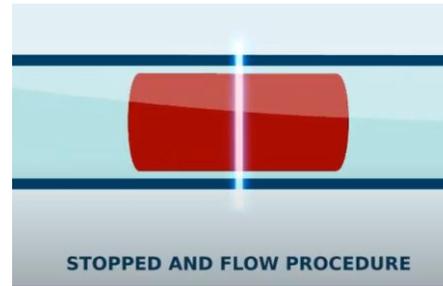

ESR

ALIFAX METHOD

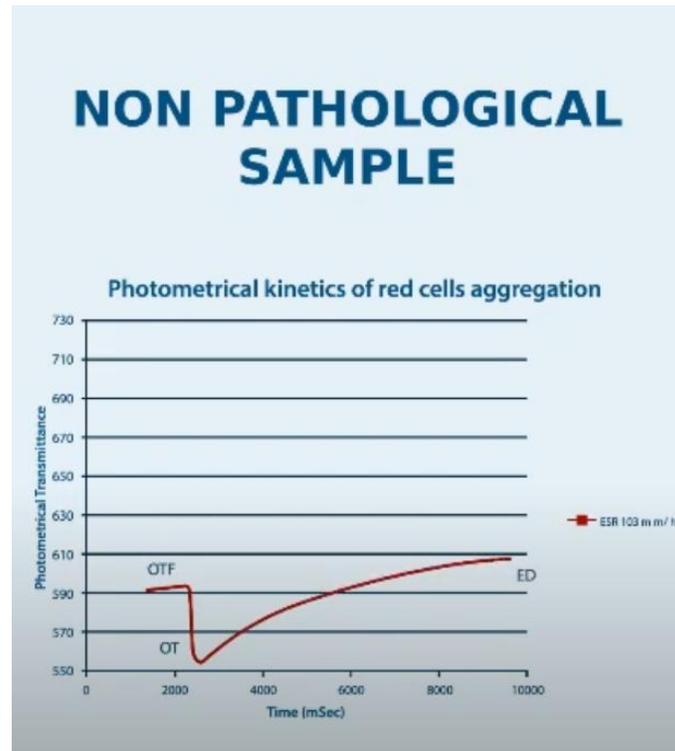


20 SECONDS





PRODOTTI A MARCHIO ALIFAX LINEA EMATOLOGIA – VES IN 20"

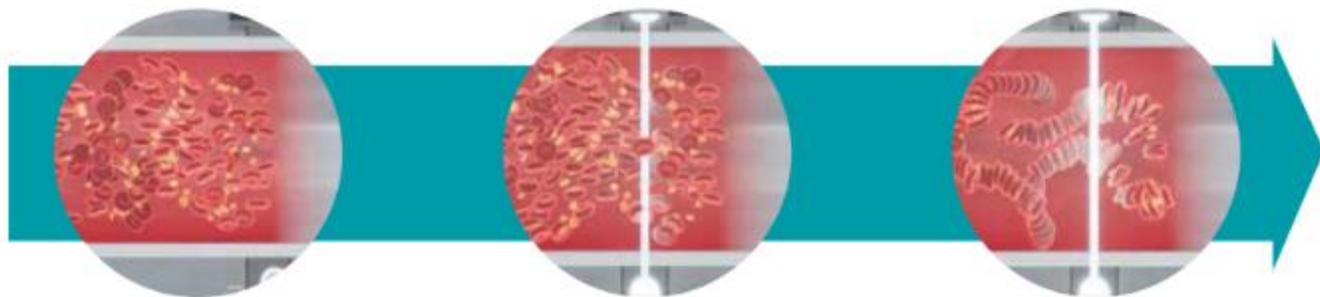



ALIFAX'S PRODUCT LINES


- ESR
- MICROBIOLOGY
- IMMUNOLOGY



GENERICO FLUSSO DIAGNOSTICO IN LABORATORIO MICROBIOLOGIA



Sample collection from the patient

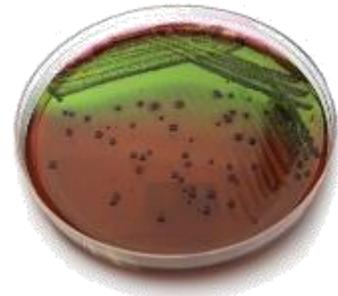

Positive sample subculture and isolation



Sample identification

Sample preparation for ID



In vitro testing of the best antibiotics panel based on microorganism ID



Day 4



Screening test result



Day 0

I segnali di scattering vengono analizzati, elaborati e convertiti in curve di crescita tracciate in **tempo reale**

L'elaborazione matematica fornisce non solo una **valutazione qualitativa della presenza/assenza di microrganismi**, ma anche una **valutazione quantitativa della quantità iniziale di batteri espressa in CFU/ml**

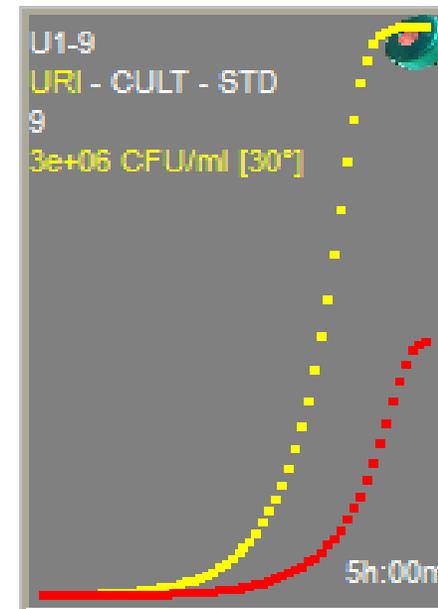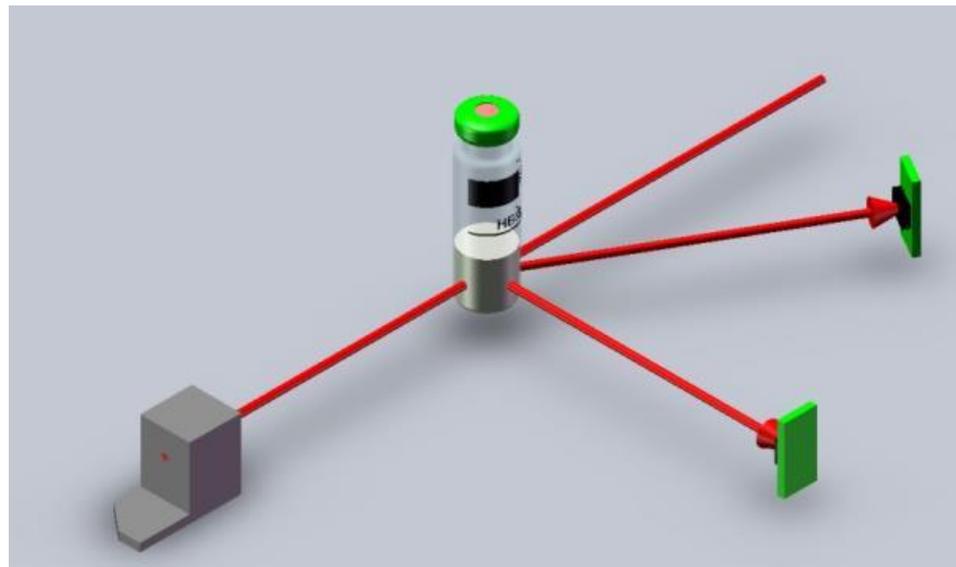

Dispersione di Rayleigh



Dispersione di luce da particelle più piccole della lunghezza d'onda

Dispersione di Brillouin



Dispersione di luce da onde sonore in un materiale

Dispersione di Thomson



Dispersione di luce da elettroni liberi



Dispersione di Mie

Dispersione di luce da particelle della lunghezza d'onda o più grandi



Dispersione di Raman

Analisi di luce da vibrazioni molecolari






Dispersione di Compton

Dispersione di luce da particelle cariche



PRODOTTI A MARCHIO ALIFAX LINEA BATTERIOLOGIA CLASSICA

- Rilevazione rapida di microorganismi in sospensione mediante letture Laser Light Scattering
- Sviluppo di tecnologie integrate per movimentazione campioni, dispensazione e semina automatica.
- Flessibilità di reagenti per lo svolgimento di molteplici test di laboratorio

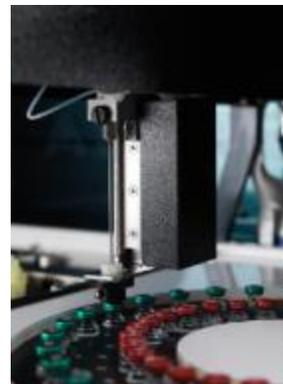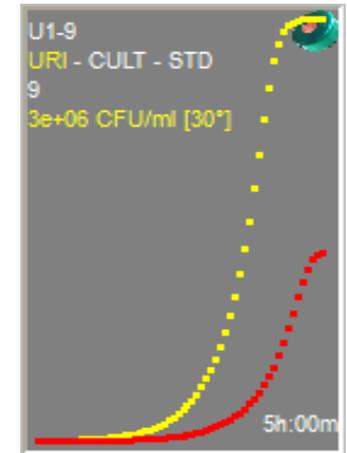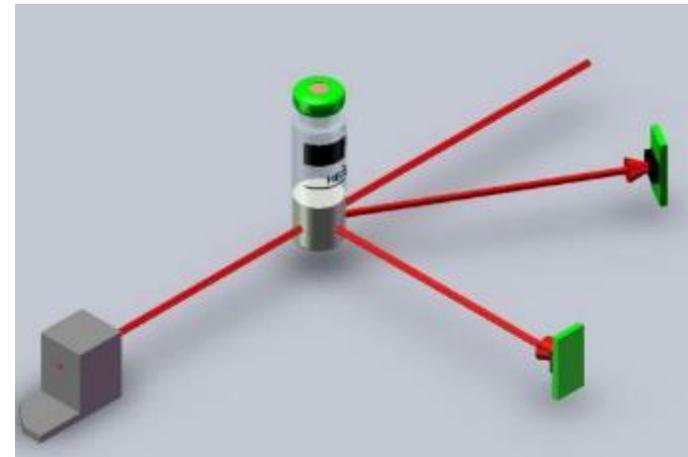

ALIFAX NEL FLUSSO DIAGNOSTICO – LINEA CLASSICA



Sample collection from the patient



Positive sample subculture and isolation



Sample identification

In vitro testing of the best antibiotics panel based on microorganism ID

Day 2

Screening test result

Sample preparation for ID

Day 0



PRODOTTI A MARCHIO ALIFAX LINEA BATTERIOLOGIA CLASSICA

TEST DI BATTERIOLOGIA



URINO COLTURA



PAR TEST



COLTURA DEI
LIQUIDI BIOLOGICI
UMANI



ANTIBIOGRAMMA



ESBL/AMPC
SCREENING



CRE SCREENING



MRSA SCREENING



ANAEROBE KIT



SABOURAUD KIT



ANTIBIOTIC RESISTANCE




5 MILLION CASES WORLDWIDE

25,000 DEATHS IN EUROPE

700,000 DEATHS WORLDWIDE

MECHANISMS OF ANTIBIOTIC ACTION

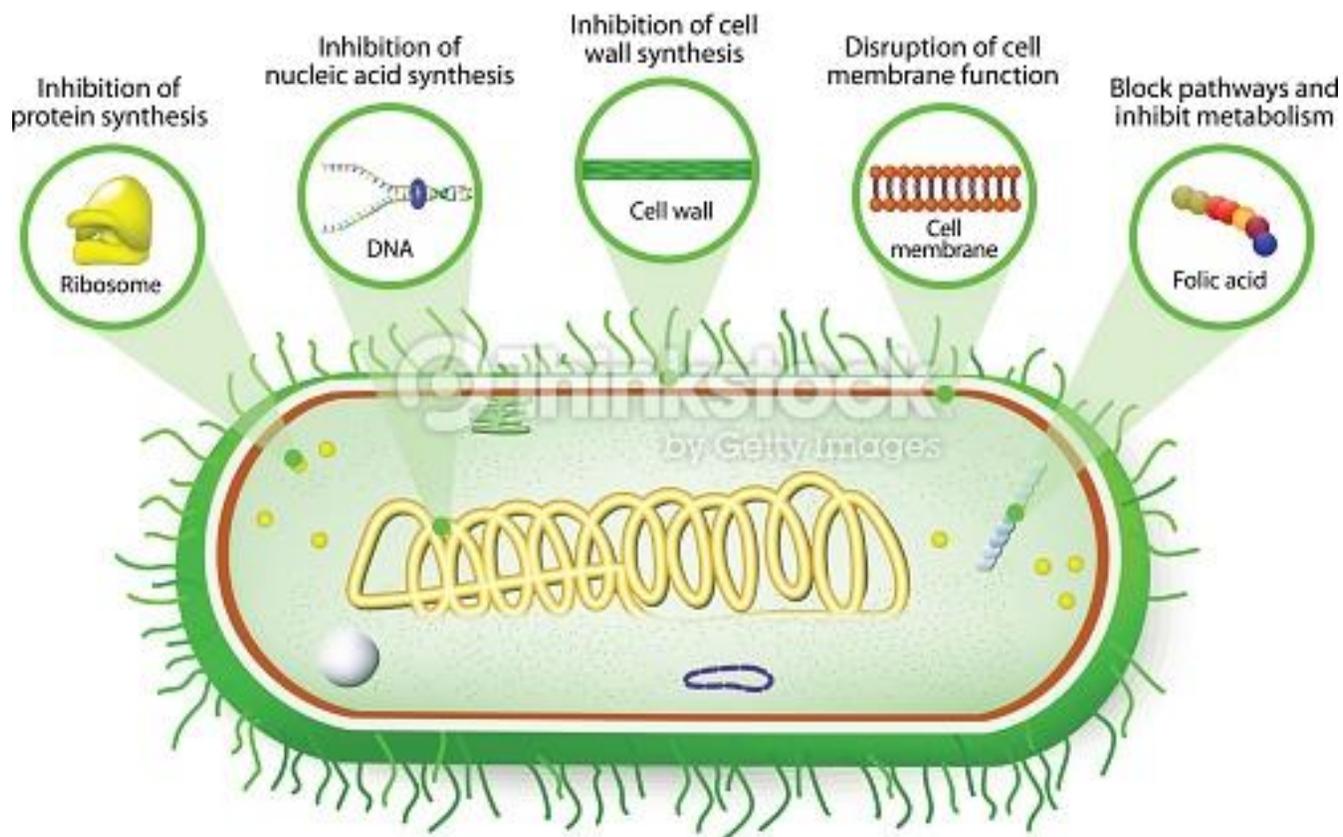

- β -lactams

- Penicillins
- β -lactam/ β -lactamase inhibitor combination
- Cephems
- Penems
- Monobactams


- Non- β -lactams

- Aminoglycosides
- Folate pathway inhibitors
- Glycopeptides
- Lipopeptides
- Macrolides
- Nitroimidazoles (only against strictly anaerobic bacteria)
- Oxazolidinones
- Quinones
- Streptogramins
- Tetracyclines
- Single-drug classes

The antibiotic resistance of bacteria is the ability to be or to become resistant to antibiotics.

May be 2 kinds:

- Intrinsic (natural)
- Acquired
 - Genetic mutation (chromosomal)
 - Antibiotic induction
 - New genes intake (esogenic)

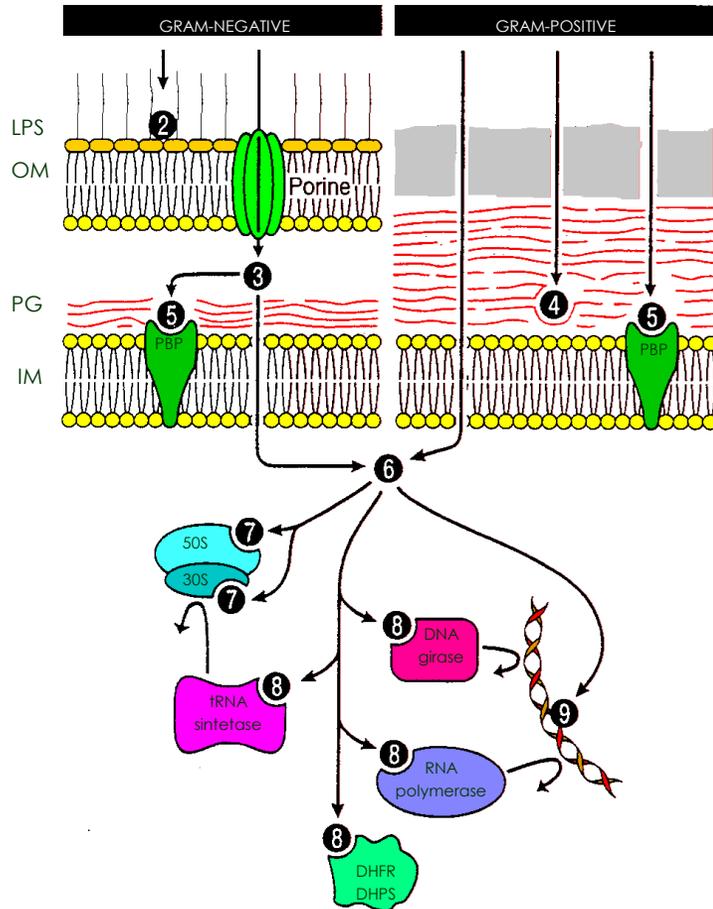

Mechanisms of resistance

The main mechanisms used by bacteria are:

- Enzymatic inactivation of drug (eg. beta-lactamase)
- Antibacterial target alteration (eg. PBP, ribosomes)
- Lower cellular permeability (eg. LPS, EPS)
- Active efflux of the drug



TIME MAGAZINE 1966 Feb 25



TIME

Subscribe

Essay: THE FUTURISTS: Looking Toward A.D. 2000

Friday, Feb. 25, 1966

Like 42

Tweet

G+ 0

Share

Read Later

(4 of 6)

Nearly all experts agree that bacterial and viral

diseases will have been virtually wiped out. Probably

arteriosclerotic heart disease will also have been

eliminated. Cells have only a few secrets still hidden

from probers, who are confident that before the year 2000 they will have found the secret that causes cancer. The

most exciting, and to some the most frightening, prospect is the chemical and electrical treatment of the brain. Dr.

Email

Print

Share

Reprints


Follow @TIME

Journal home > Archive > insight > Full text > Figure 2

FIGURE 2. Leading causes of death worldwide.

From the following article:
The challenge of emerging and re-emerging infectious diseases
 David M. Morens, Gregory K. Folkers & Anthony S. Fauci
Nature **430**, 242-249(8 July 2004)
 doi:10.1038/nature02759

[back to article](#)

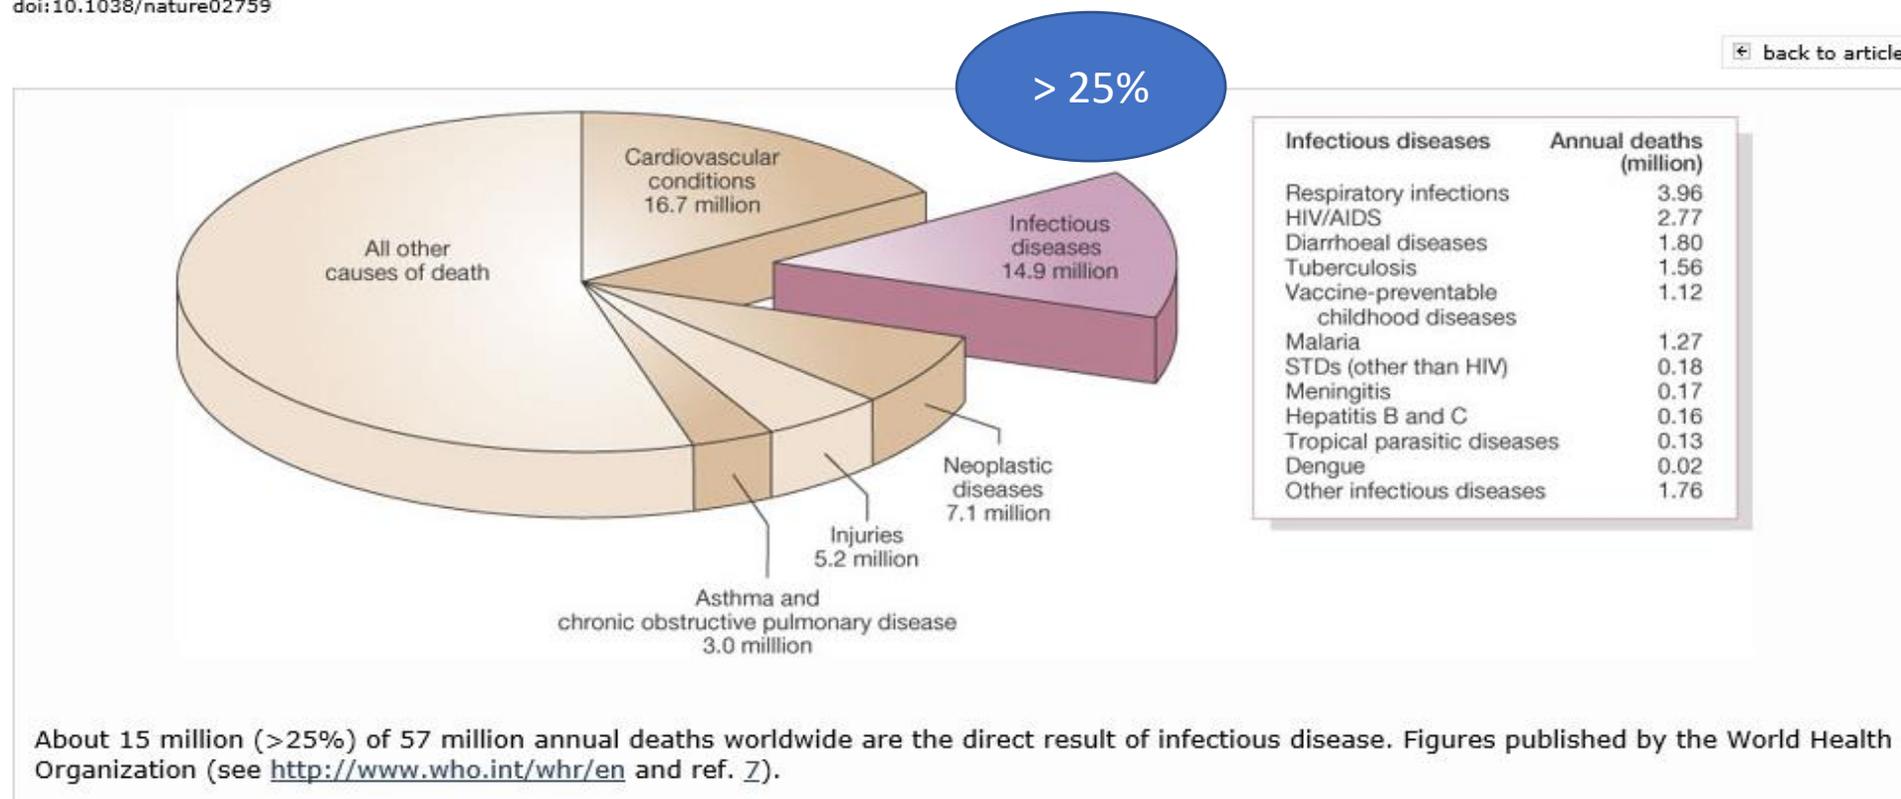

About 15 million (>25%) of 57 million annual deaths worldwide are the direct result of infectious disease. Figures published by the World Health Organization (see <http://www.who.int/whr/en> and ref. 7).

Nature 2004

	Resistant Pathogen	2017 Threat Estimate	2018 Threat Estimate	2019 Threat Estimate	2017-2019 Change	2020 Threat Estimate and 2019-2020 Change
URGENT	Carbapenem-resistant <i>Acinetobacter</i>	8,500 cases 700 deaths	6,300 cases 500 deaths	6,000 cases 500 deaths	Stable*	7,500 cases 700 deaths Overall: 55% increase* Hospital-onset: 78% increase*
	Antifungal-resistant <i>Candida auris</i>	171 clinical cases†	329 clinical cases	466 clinical cases	Increase	754 cases Overall: 60% increase
	<i>Clostridioides difficile</i>	223,900 infections 12,800 deaths	221,200 infections 12,600 deaths	202,600 infections 11,500 deaths	Decrease	Data delayed due to COVID-19 pandemic
	Carbapenem-resistant Enterobacterales	13,100 cases 1,100 deaths	10,300 cases 900 deaths	11,900 cases 1,000 deaths	Decrease*	12,700 cases 1,100 deaths Overall: Stable* Hospital-onset: 35% increase*
	Drug-resistant <i>Neisseria gonorrhoeae</i>	550,000 infections	804,000 infections	942,000 infections	Increase	Data unavailable due to COVID-19 pandemic
SERIOUS	Drug-resistant <i>Campylobacter</i>	448,400 infections 70 deaths	630,810 infections	725,210 infections	Increase	Data delayed due to COVID-19 pandemic† 26% of infections were resistant, a 10% decrease
	Antifungal-resistant <i>Candida</i>	34,800 cases 1,700 deaths	27,000 cases 1,300 deaths	26,600 cases 1,300 deaths	Decrease*	28,100 cases 1,400 deaths Overall: 12% increase* Hospital-onset: 26% increase*
	ESBL-producing Enterobacterales	197,400 cases 9,100 deaths	174,100 cases 8,100 deaths	194,400 cases 9,000 deaths	Increase*	197,500 cases 9,300 deaths Overall: 10% increase* Hospital-onset: 32% increase*
	Vancomycin-resistant Enterococcus	54,500 cases 5,400 deaths	46,800 cases 4,700 deaths	47,000 cases 4,700 deaths	Stable*	50,300 cases 5,000 deaths Overall: 10% increase* Hospital-onset: 14% increase*



SERIOUS

CONCERNING

Resistant Pathogen	2017 Threat Estimate	2018 Threat Estimate	2019 Threat Estimate	2017-2019 Change	2020 Threat Estimate and 2019-2020 Change
Multidrug-resistant <i>Pseudomonas aeruginosa</i>	32,600 cases 2,700 deaths	29,500 cases 2,500 deaths	28,200 cases 2,400 deaths	Decrease*	28,800 cases 2,500 deaths Overall: Stable* Hospital-onset: 32% increase*
Drug-resistant nontyphoidal <i>Salmonella</i>	212,500 infections 70 deaths	228,290 infections	254,810 infections	Increase	Data delayed due to COVID-19 pandemic† 14% of infections were resistant, a 3% decrease
Drug-resistant <i>Salmonella</i> serotype Typhi	4,100 infections <5 deaths	4,640 infections	6,130 infections	Increase	Data delayed due to COVID-19 pandemic† 85% of infections were resistant, a 10% increase
Drug-resistant <i>Shigella</i>	77,000 infections <5 deaths	215,850 infections	242,020 infections	Increase	Data delayed due to COVID-19 pandemic† 46% of infections were resistant, a 2% increase
Methicillin-resistant <i>Staphylococcus aureus</i>	323,700 cases 10,600 deaths	298,700 cases 10,000 deaths	306,600 cases 10,200 deaths	Stable*	279,300 cases 9,800 deaths Overall: Stable* Hospital-onset: 13% increase*
Drug-resistant <i>Streptococcus pneumoniae</i>	12,100 invasive infections 1,500 deaths†	See pathogen page if comparing data over time	12,000 invasive infections 1,200 deaths	Stable	Data delayed due to COVID-19 pandemic
Drug-resistant Tuberculosis (TB)	888 cases 73 deaths†	962 cases 102 deaths	919 cases	Stable	661 cases Decrease†
Erythromycin-resistant group A <i>Streptococcus</i>	5,400 infections 450 deaths†	See pathogen page if comparing data over time	6,200 infections 560 deaths	Increase	Data delayed due to COVID-19 pandemic
Clindamycin-resistant group B <i>Streptococcus</i>	13,000 infections 720 deaths†	See pathogen page if comparing data over time	15,300 cases 940 deaths	Increase	Data delayed due to COVID-19 pandemic

MDR Bacteria Responsible of Hospital Aquired Infections


- E:** *Enterococcus faecium*
- S:** *Staphylococcus aureus*
- K:** *Klebsiella pneumoniae*
- A:** *Acinetobacter baumannii*
- P:** *Pseudomonas aeruginosa*
- E:** *Enterobacter species*



World Health Organization (WHO) list, 2017

MDRO infections represent a growing global health problem, further intensified in recent years by the pandemic, which due to an unpredictable emergency has increased the selective pressure and decreased the active surveillance in the hospital environment.

Alarming increase in resistant infections during hospitalization from 2019 to 2020*

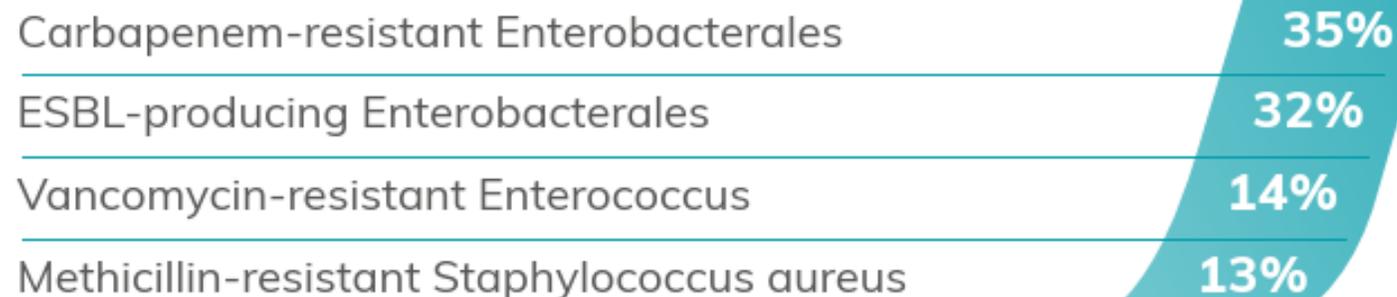

It is more urgent than ever to prioritize efforts towards resistance containment and support the One Health program to improve the detection, characterization and rapid response to emerging AMR.

* COVID-19: U.S. Impact on Antimicrobial Resistance, Special Report 2022

ANTIBIOTIC RESISTANCE?

IT'S AN ONGOING PROCESS WITH A DRAMATIC ESCALATION

MDR: Multi Drug Resistance



THE WORST SCENARIO:

XDR: Extensive Drug Resistance


RESISTANCE TO ALL ANTIBIOTICS, EXCEPT 1 OR 2

PDR: Pan Drug Resistance

RESISTANCE TO ALL ANTIBIOTICS

WHY IS ANTIMICROBIAL RESISTANCE A GLOBAL CONCERN?


Deaths attributable to antimicrobial resistance every year by 2050

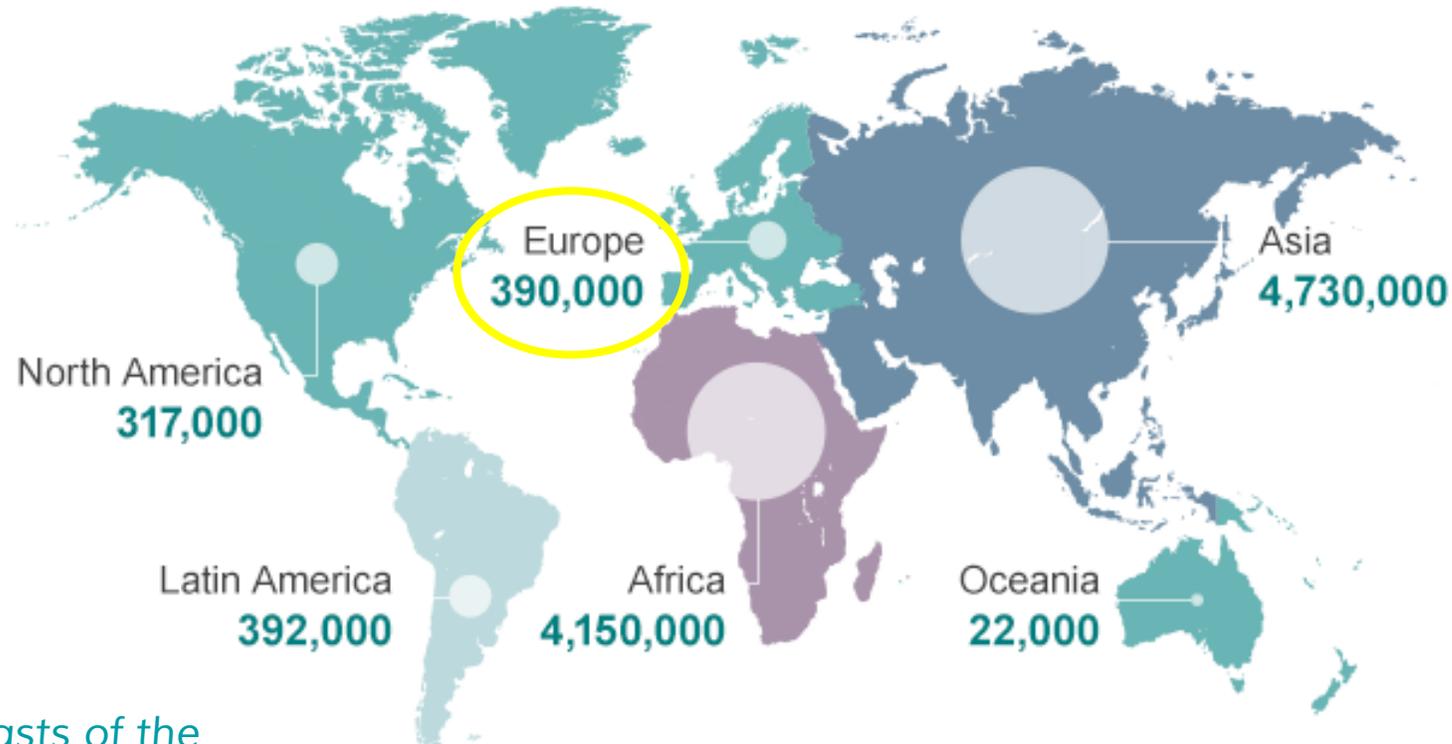

2.4 Million people could lose their lives in Europe, North America And Australia in the period 2015-2050. According to the forecasts, Italy, Greece and Portugal would rank among the top of OCSE countries for the highest mortality rates from AMR

According to the forecasts of the World Bank, the economic impact of the AMR could exceed that of the financial crisis of 2008-2009.


MRSA METHICILLIN-RESISTANT STAPHYLOCOCCUS AUREUS

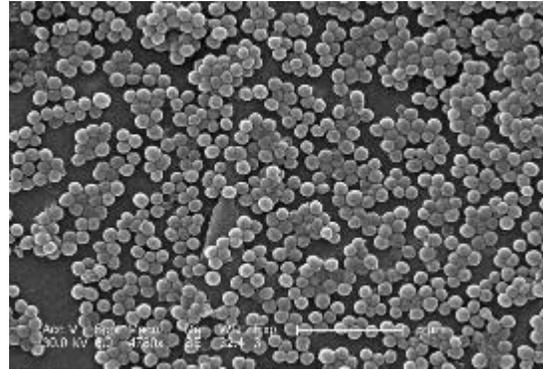

People with methicillin-resistant *Staphylococcus aureus* infections are 64% more likely to die than people with drug-sensitive infections (WHO 2020)


GOLD STANDARD:

Chromogenic selective media culture from nasal, throat, inguinal swab (direct or enriched) + Confirmation Test

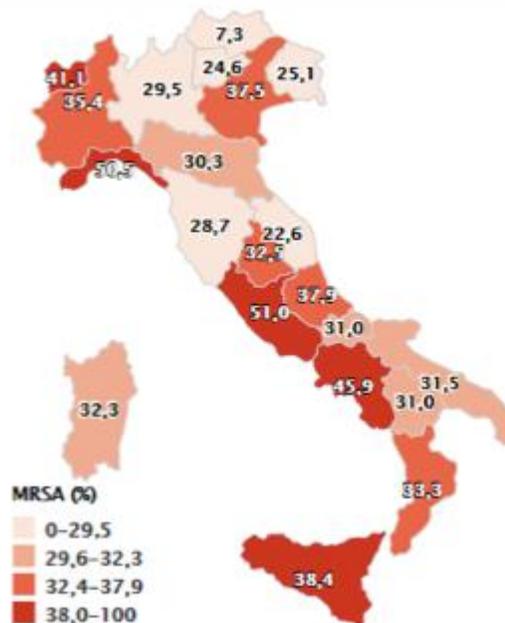


TURN AROUND TIME (TTR):
24h, 48h, and 72h

CPE CARBAPENEMASE-PRODUCING ENTEROBACTERIALES

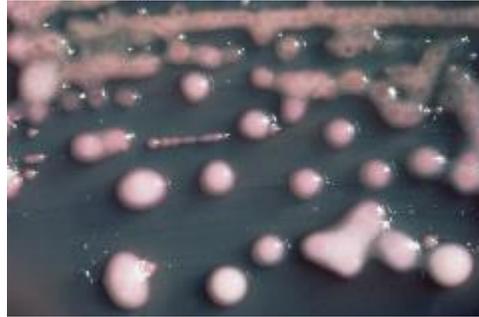


Resistance in carbapenem antibiotics treatment has spread to all regions of the world. They are a major cause of hospital-acquired infections such as pneumonia, bloodstream infections, and infections in newborns and intensive-care unit patients. In some countries, such as in some region of Italy, carbapenem antibiotics do not work in more than half of the patients treated due to infections with resistant microorganisms.

GOLD STANDARD:
Chromogenic selective media culture from rectal swab + Confirmation Test

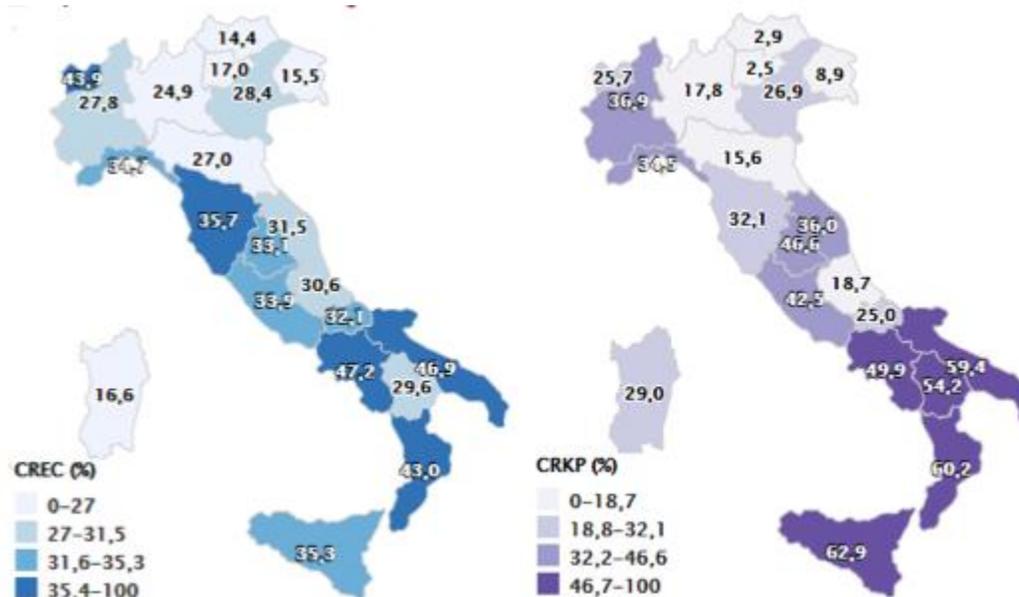

TURN AROUND TIME (TTR):
24h, 48h, and 72h

MDRO Cycle of Transmission

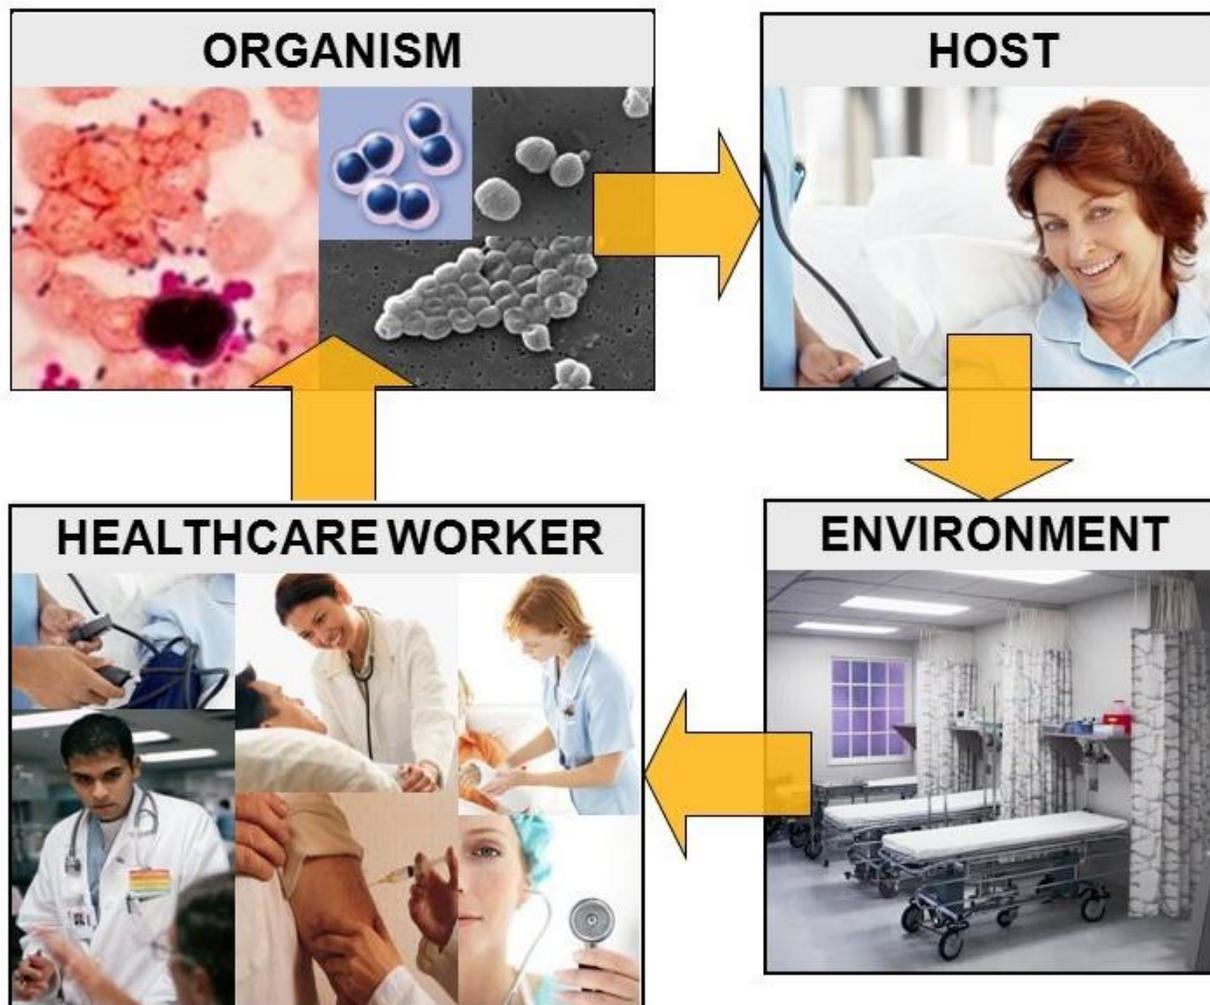

MDRO spreading induces:

- Higher mortality in critical settings;
- Increased hospitalizations;
- Higher costs of patient management

ANTIMICROBIAL STEWARDSHIP



CAUSE DELLE RESISTENZE ANTIMICROBICHE



**ECESSO
DI PRESCRIZIONI
DI ANTIBIOTICO**



**MANCATA ADERENZA
ALLA TERAPIA
PRESCRITTA**



**ABUSO DI ANTIBIOTICI
IN ALLEVAMENTO**



**RIDOTTO
CONTROLLO
DELLE INFEZIONI
OSPEDALIERE**



**SCARSA
OSSERVANZA
DELLE REGOLE
DI IGENE**




**CARENZA DI
METODOLOGIE
DIAGNOSTICHE
RAPIDE EFFICACI**

NEW CDC DATA


MORE THAN HALF OF ANTIBIOTIC PRESCRIBING FOR SELECTED EVENTS IN HOSPITALS WAS NOT CONSISTENT WITH RECOMMENDED PRESCRIBING PRACTICES




ANTIBIOTIC PRESCRIBING WAS NOT SUPPORTED IN:




with community-acquired pneumonia



with urinary tract infections



prescribed fluoroquinolone treatment



prescribed intravenous vancomycin antibiotic

HOSPITAL PRESCRIBERS & PHARMACISTS CAN IMPROVE PRESCRIBING:



Optimize antibiotic selection



Re-assess antibiotic treatment when the results of diagnostic testing are available



Use the shortest effective duration of therapy


FIND RESOURCES ON HOW TO IMPROVE HOSPITAL ANTIBIOTIC USE AND HELP FIGHT ANTIBIOTIC RESISTANCE:

<https://bit.ly/HospitalCoreElements>

Mortality Risk with Increasing Delays in Initiation of Effective Antimicrobial Therapy

Give the right therapy in a short time could save the life of the critical patient

In the case of systemic bacterial infections, **the time for the diagnosis is a decisive factor for the survival of the patient** since the delay of adequate antibiotic therapy increases the likelihood of patient death of **7.5% for each hour of delay and exponentially after 24 hours** after the onset of hypotension (Kumar, Crit Care Med 2006; 34: 1589-96).

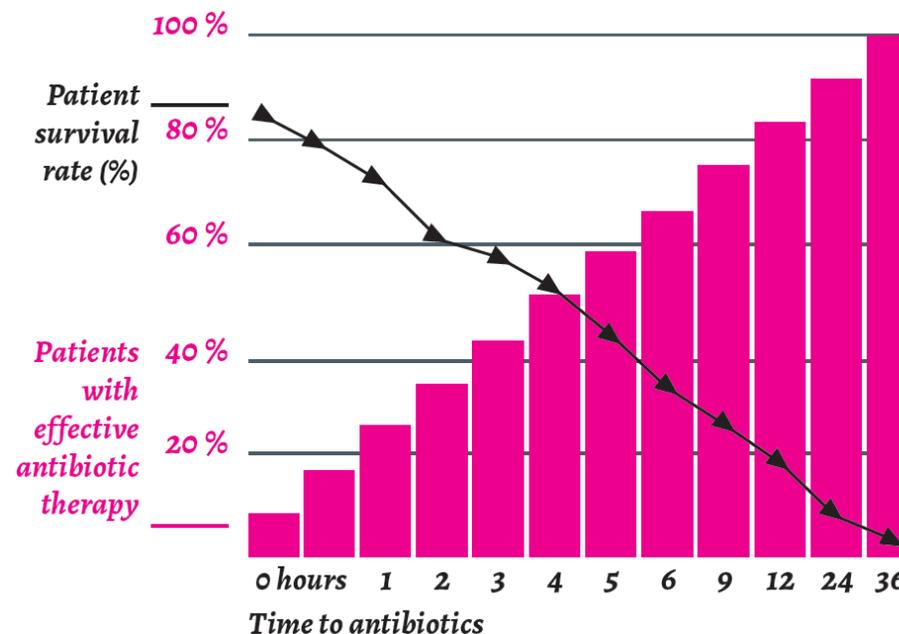

CONFIDENTIAL DOCUMENT: FOR PRIVATE USE ONLY, DO NOT DISCLOSE




Sample collection from the patient



Positive sample subculture and isolation



Sample identification

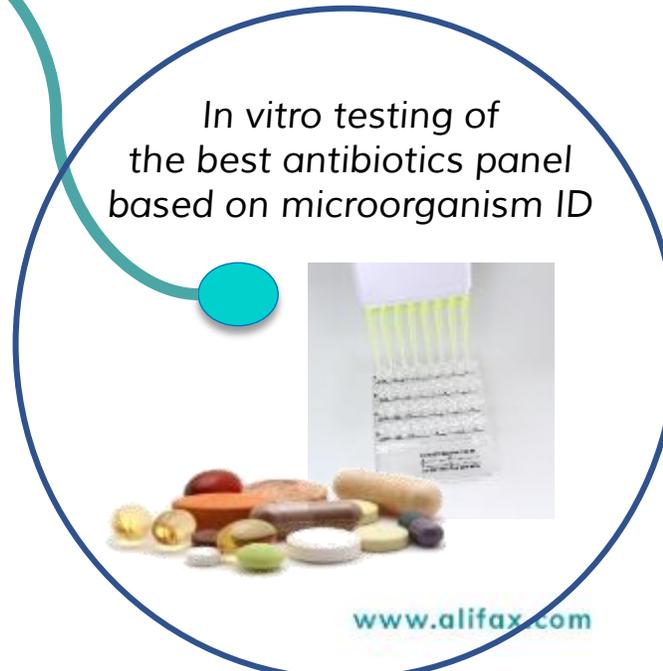

In vitro testing of the best antibiotics panel based on microorganism ID

Day 4


Day 0

Screening test result


Sample preparation for ID



ANTIBIOGRAMMA E MIC

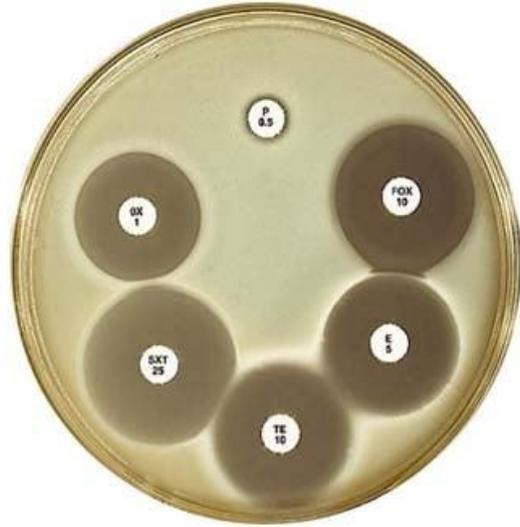

Sia test qualitativi che quantitavi per l'esecuzione dell'antibiogramma richiedono un'incubazione O/N

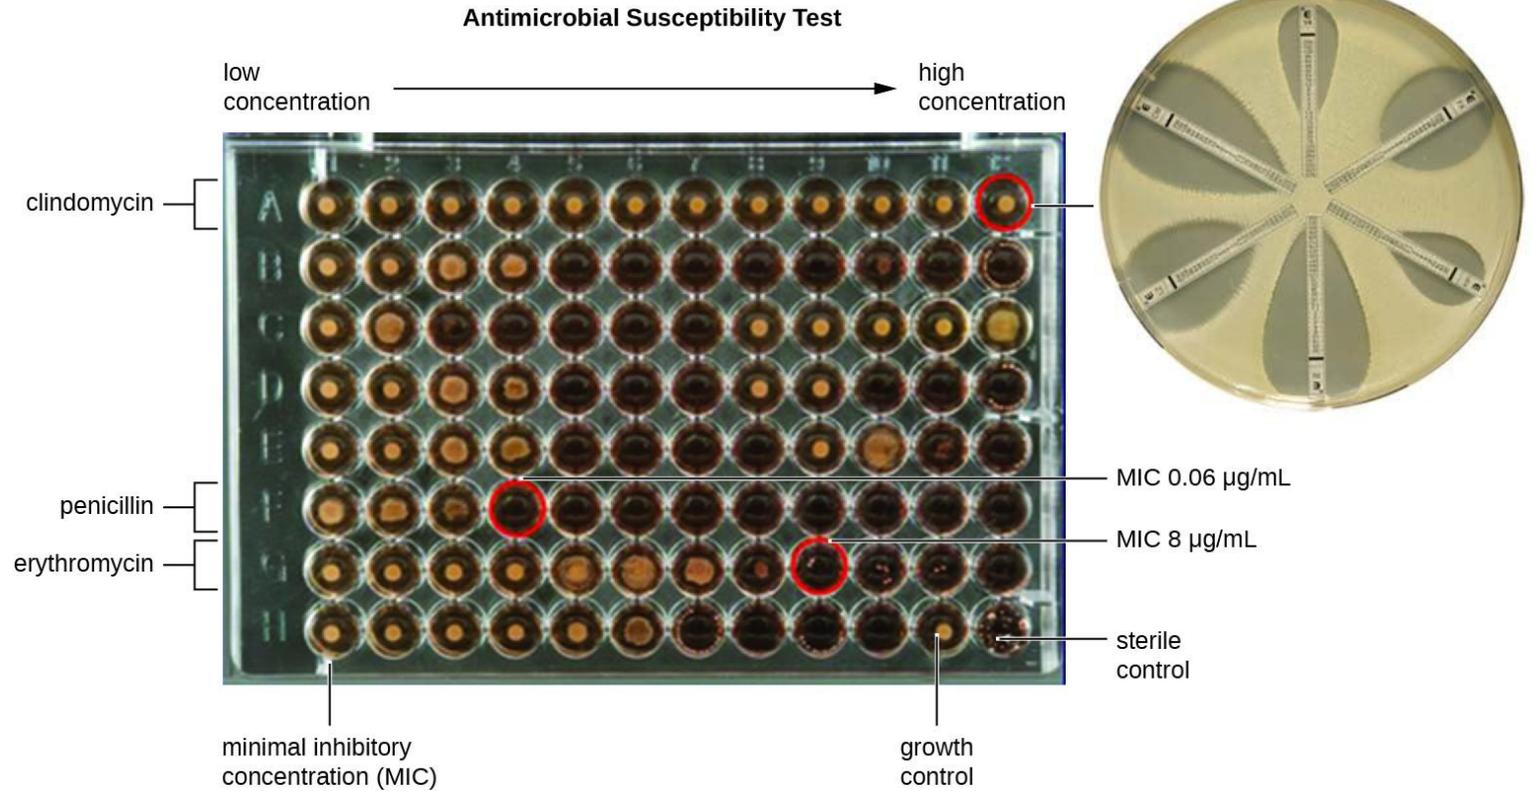

GESTIONE DEL PAZIENTE CRITICO SELEZIONE TERAPEUTICA

- Valutazione rapida delle migliori scelte terapeutiche per il paziente critico grazie alla tecnologia Laser Light Scattering




RISULTATI IN SOLE 3/5 ORE

"la correlazione con i metodi di riferimento è del 97%" (14)

REPORT	PIC %
Sensibile	50-0%
Intermedio	65-50%
Resistente	65-100%

I risultati sono espressi in percentuale di resistenza agli antibiotici (PIC) e classificati come: Resistenti, Intermedi o Sensibili

100 µl di sospensione 0.5 McFarland + 200 µl di antibiotico

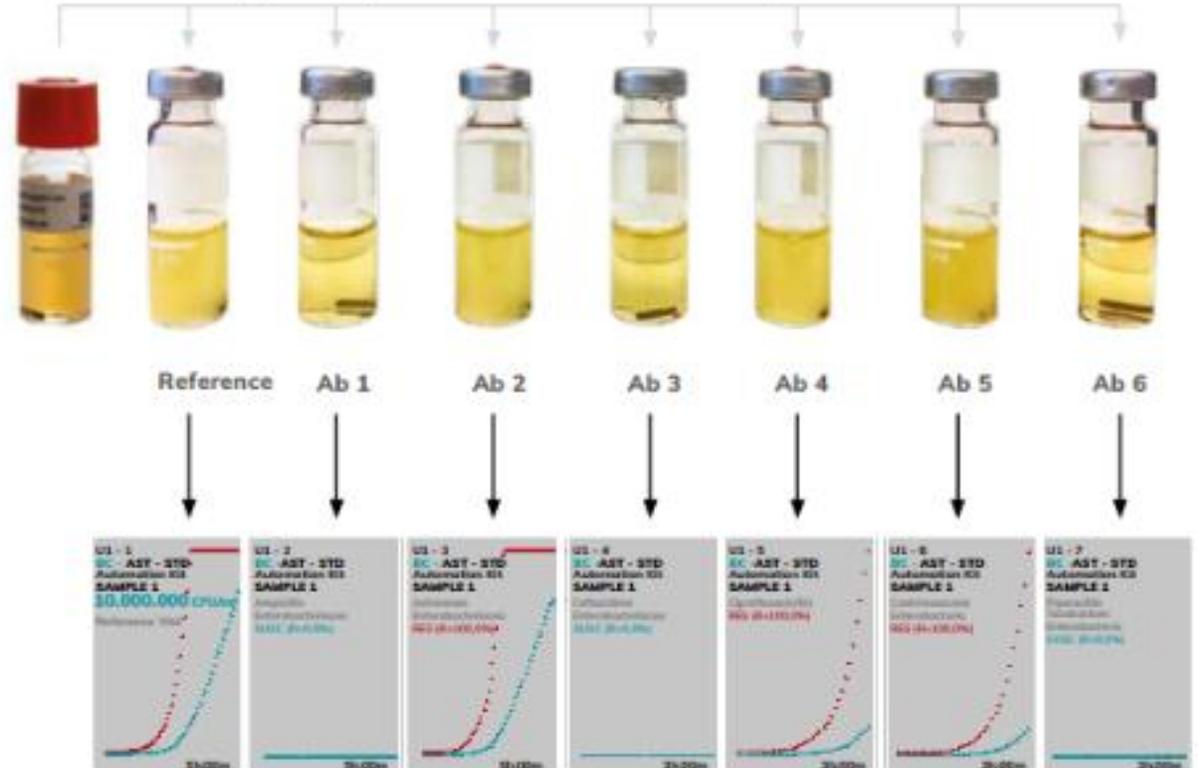



	RAP SEPSIS Fenotipico	TRADITIONAL AST Fenotipico	BIOLOGIA MOLECOLARE Genotipico
Turnaround time (TAT)	3 o 5 ore	48-72 ore	1-2 ore
Report	Sensibile e resistente	Sensibile e resistente	Solo le resistenze note
Utilità dei risultati	RAP SEPSIS Fornisce risultati clinici rilevanti	Utile per la conferma definitiva e per gli studi epidemiologici	Risultati clinicamente utili SOLO per le resistenze note, non info sulla sensibilità
Pannelli di antibiotici	PERSONALIZZABILE per il paziente	Pannelli	Non applicabile
Automazione	Sistema di inoculo Walk-away, McFarland e lettura	Lettura Semi-automatica	Semi-automatico
Costi	€€€	€€	€€€€€

ALIFAX NEL FLUSSO DIAGNOSTICO – LINEA CLASSICA



Sample collection from the patient



Positive sample subculture and isolation



Sample identification


In vitro testing of the best antibiotics panel based on microorganism ID

Day 2


Screening test result

Sample preparation for ID

Day 0





ALIFAX NEL FLUSSO DIAGNOSTICO – NUOVA GENERAZIONE PRODOTTI

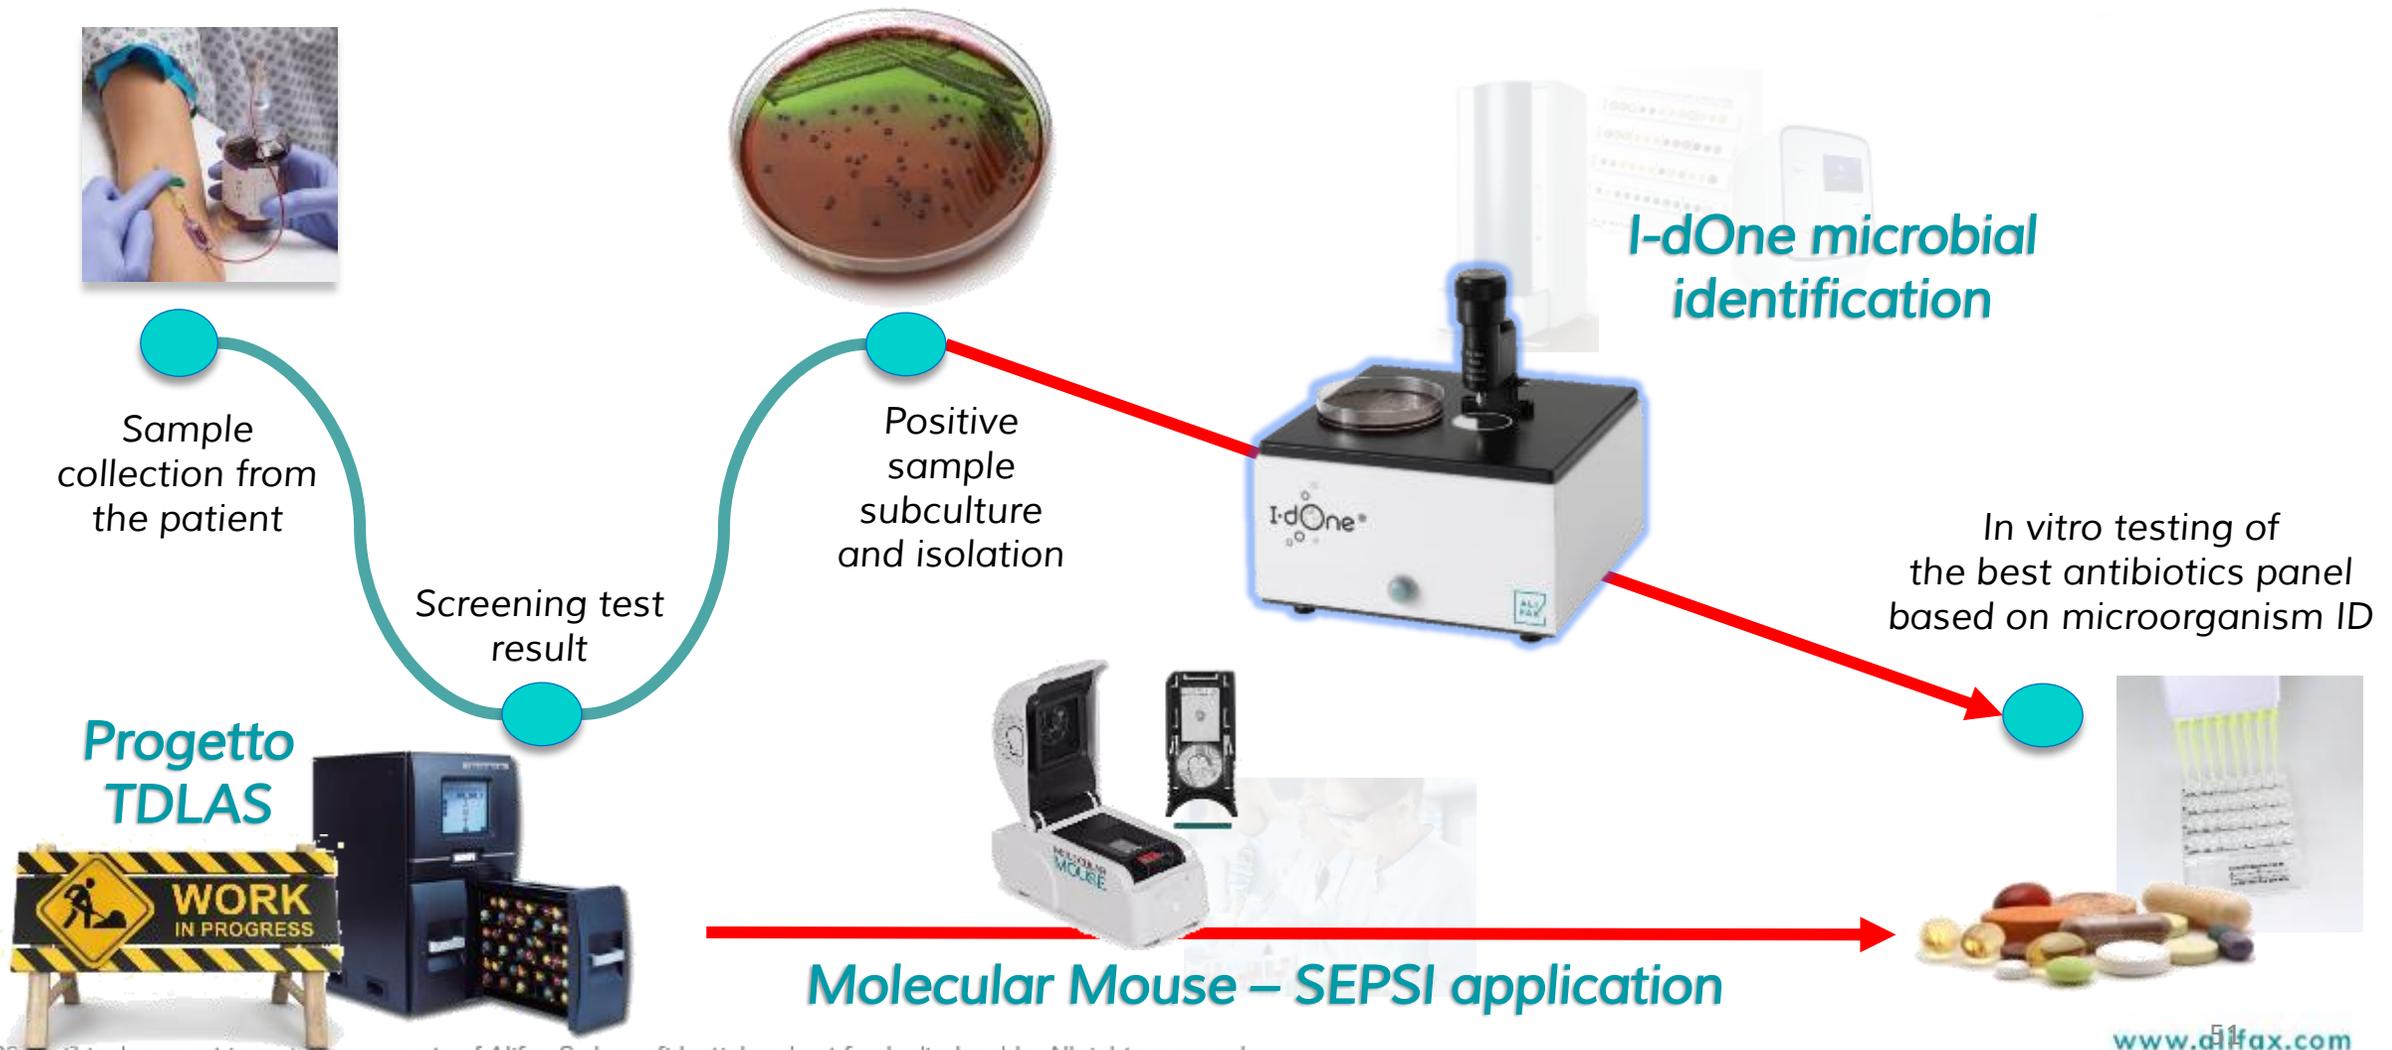

1. *General introduction about Alifax R&D and Design*
2. *Main areas of interest in Alifax*
 - a) *ESR (scope of the test, biological mechanisms, clinical importance)*
 - b) *Microbiology (Antimicrobial Stewardship, MDROs, Clinical microbiology workflow)*
 - c) *Introduction of new products in the market*
- 3. Design process (Project Vision, Stakeholder needs, Usability, Safety, Performance)**
4. *From Design to Manufacturing and Sells: Process Validation, Safety, Registrations*

ALIFAX NEL FLUSSO DIAGNOSTICO NUOVE APPLICAZIONI

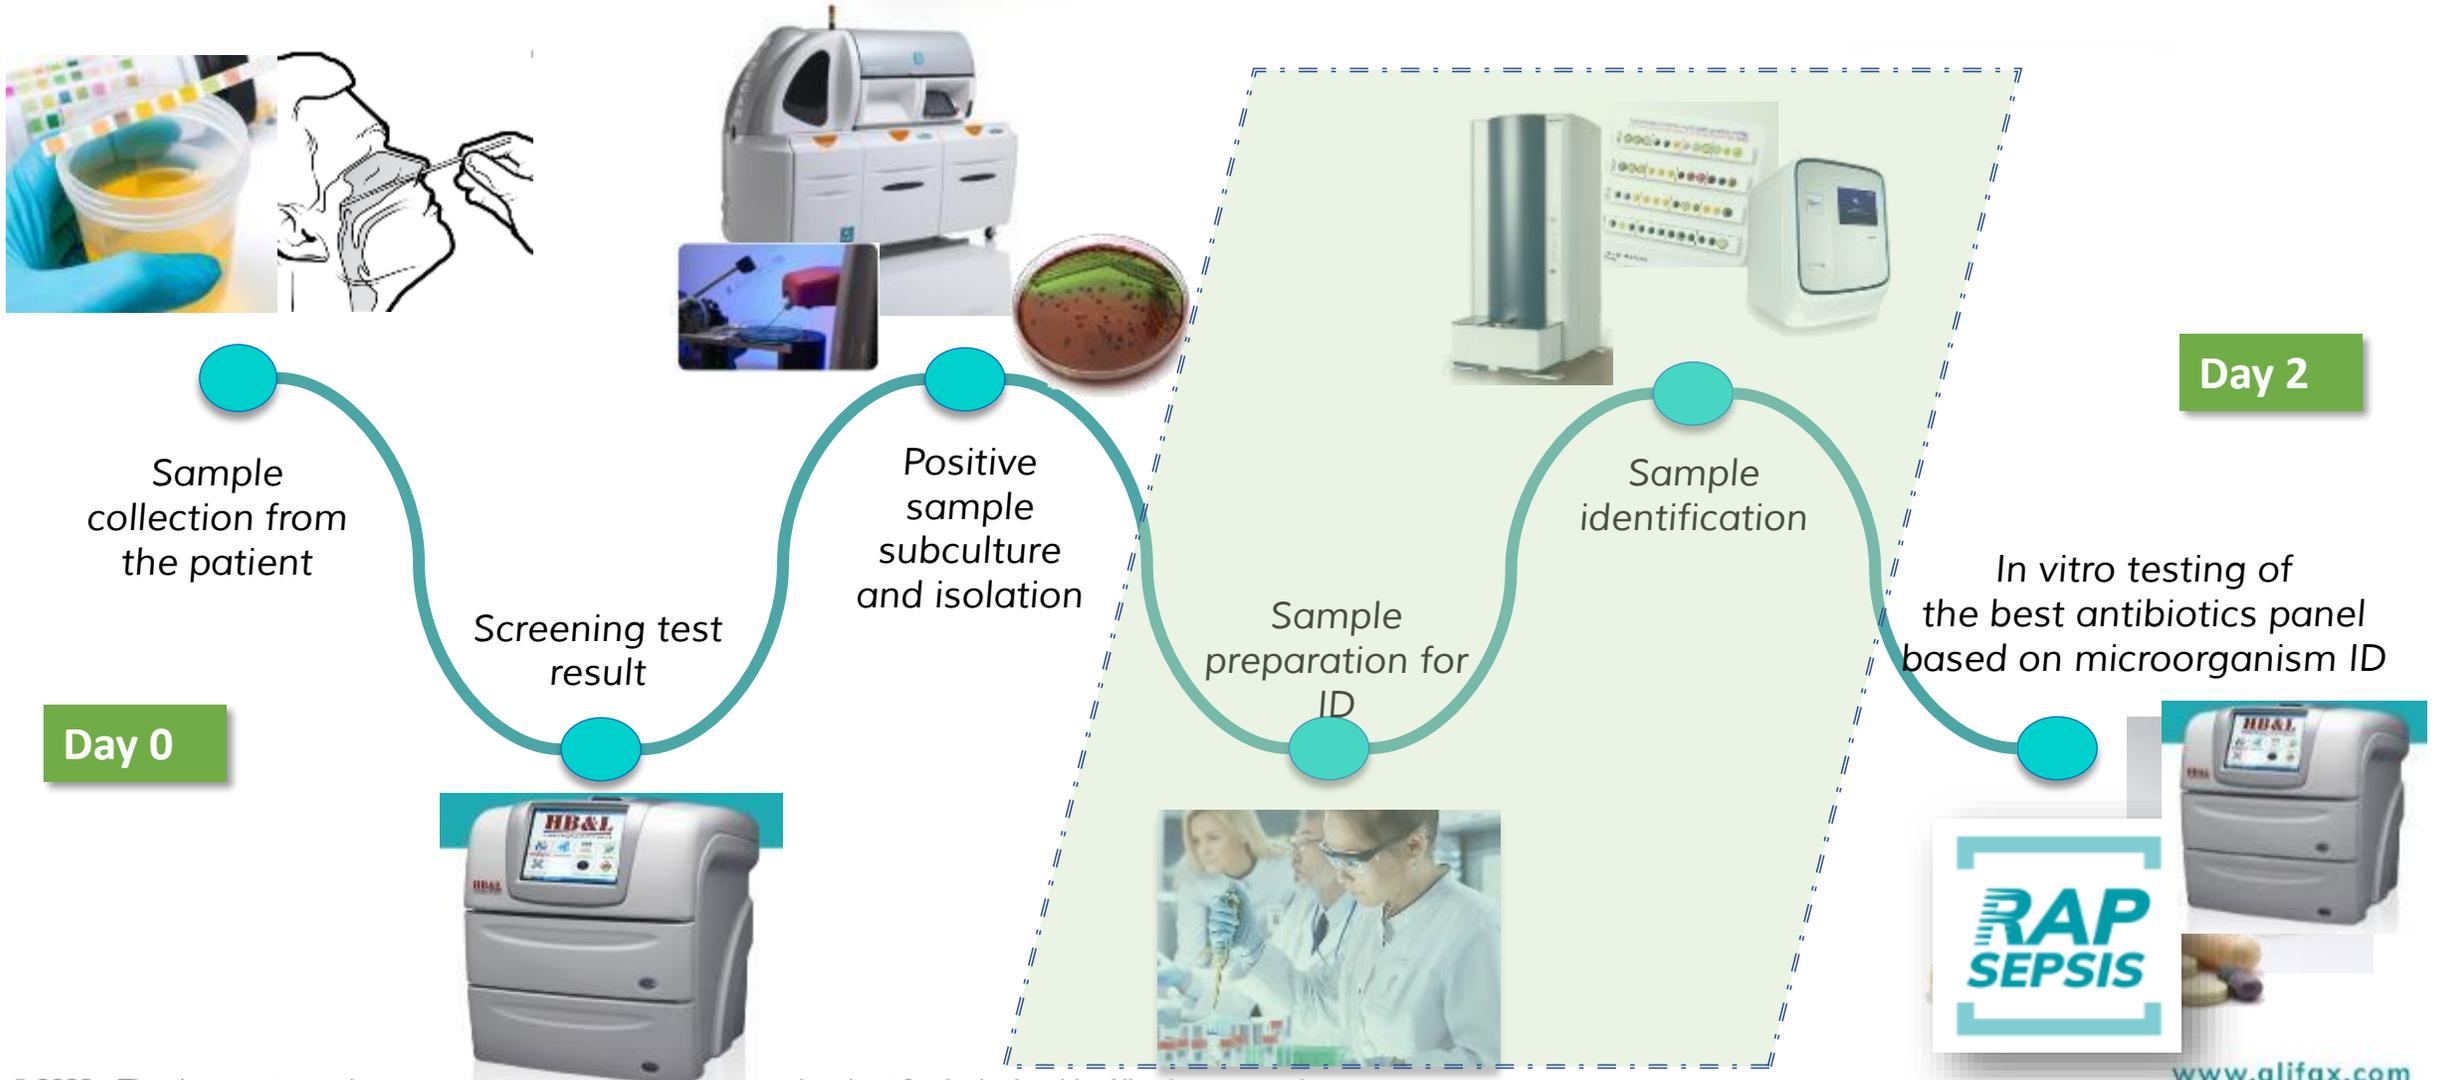

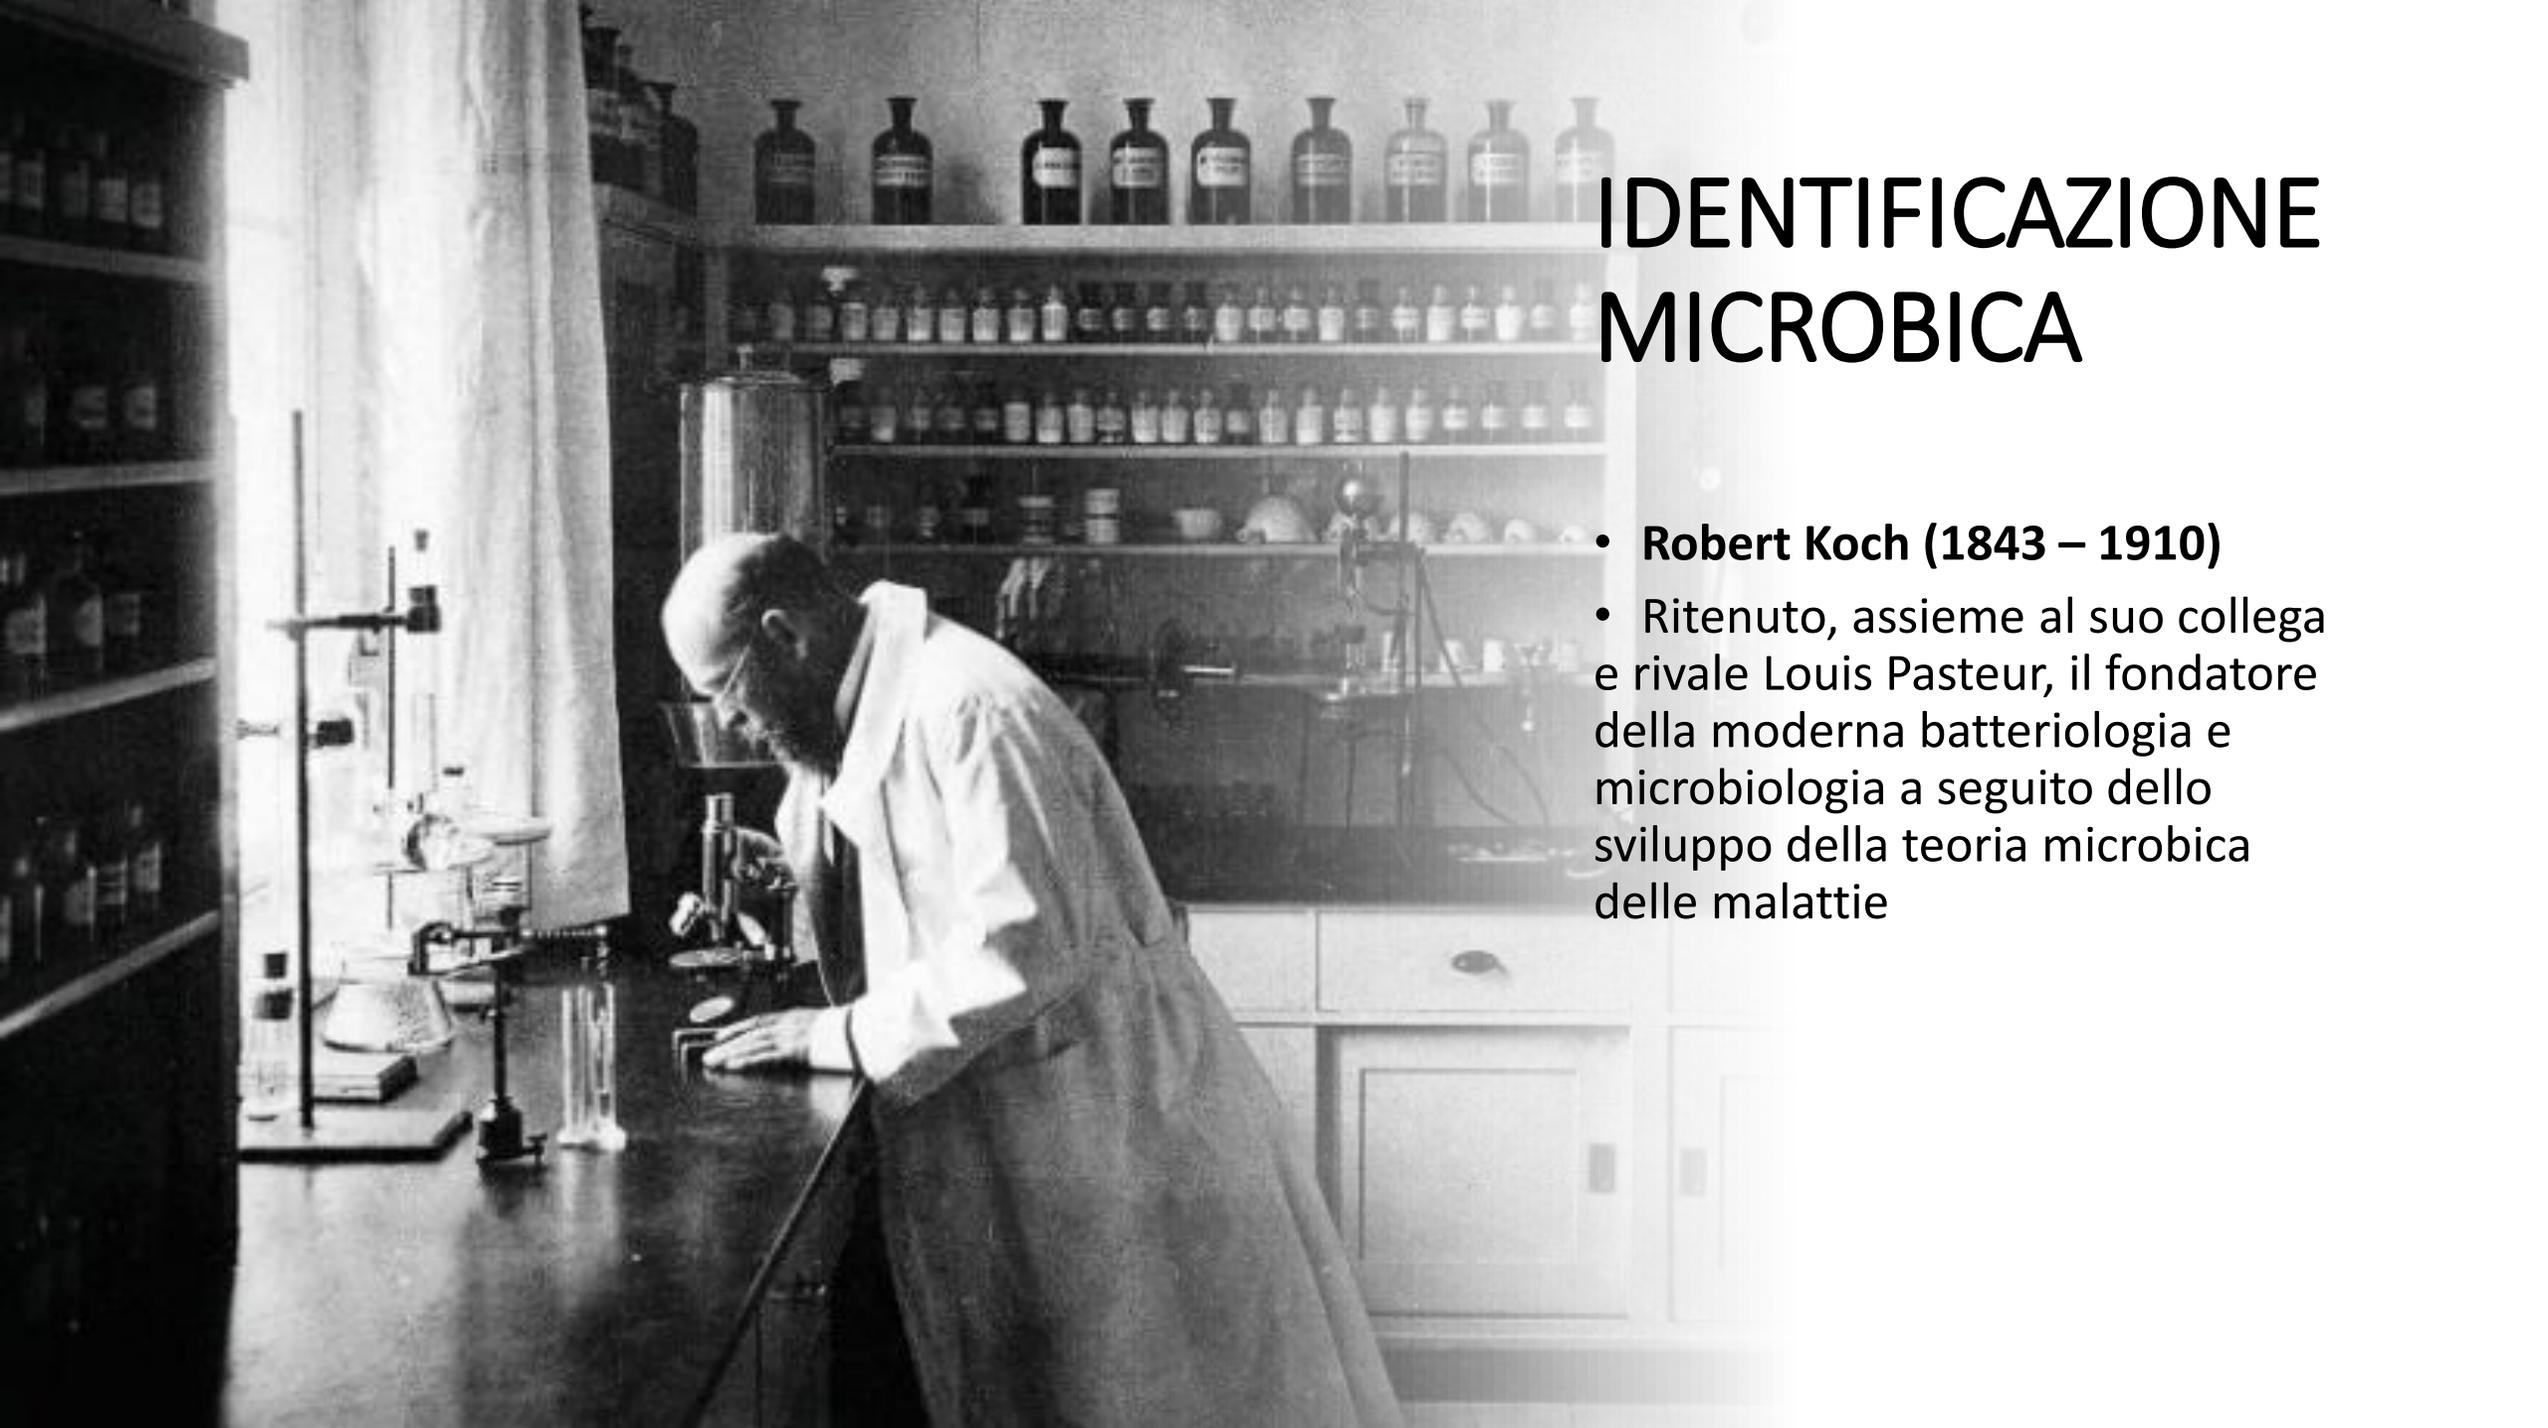


IDENTIFICAZIONE MICROBICA

- **Robert Koch (1843 – 1910)**
- Ritenuto, assieme al suo collega e rivale Louis Pasteur, il fondatore della moderna batteriologia e microbiologia a seguito dello sviluppo della teoria microbica delle malattie

IDENTIFICAZIONE MICROBICA - VISIVA










Form

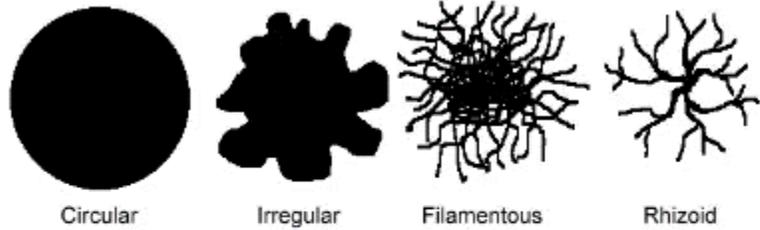


Elevation



Margin

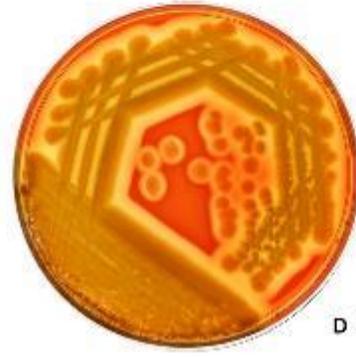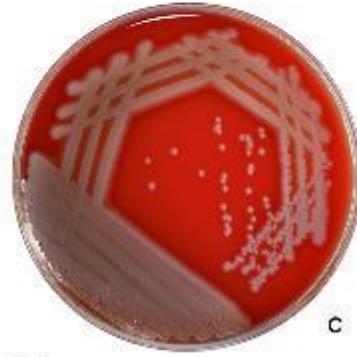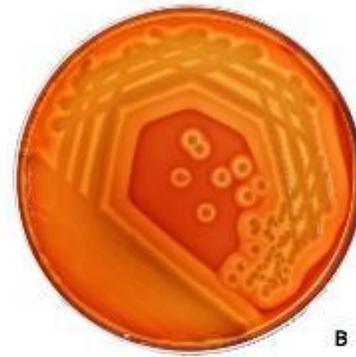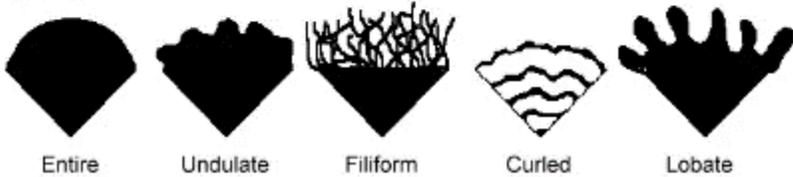

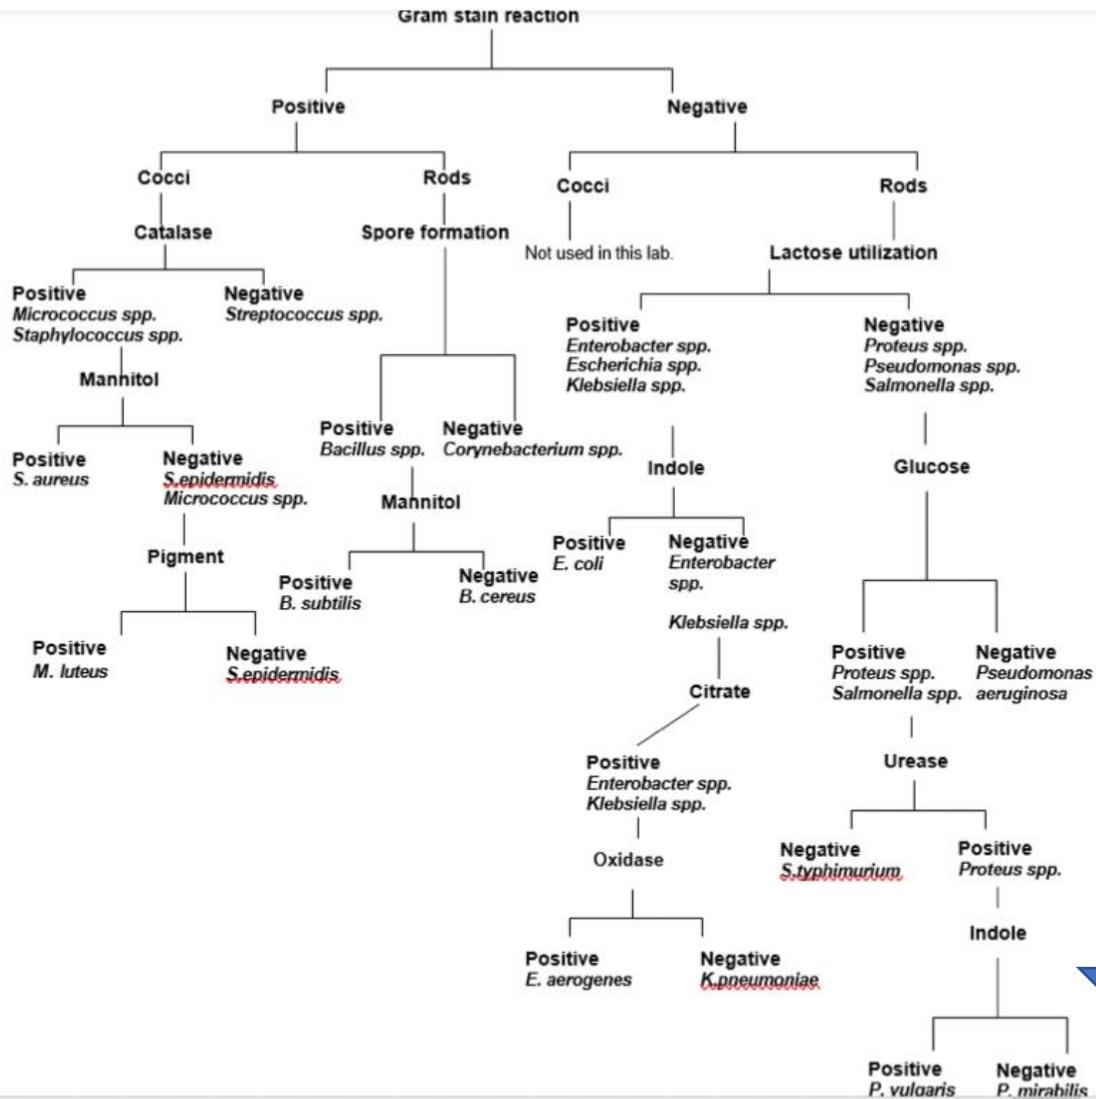


Giorni / Settimane


Test Biochimici eseguiti in funzione di algoritmi di identificazione basati su letteratura. Metodo macchinoso, time-consuming e molto pronò ad errori


BIOCHEMICAL REACTIONS OF E.coli



IMViC series - Escherichia coli

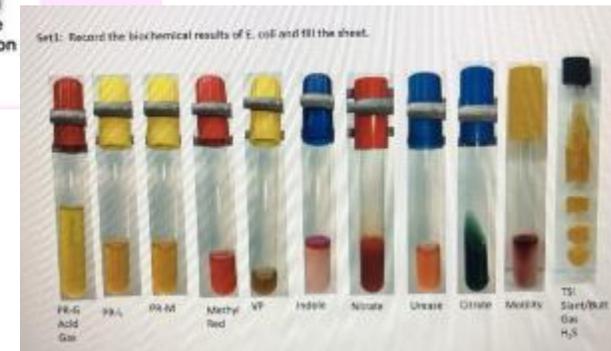

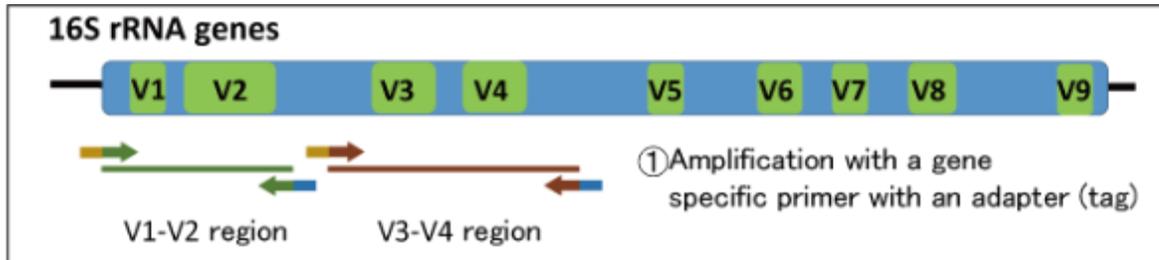


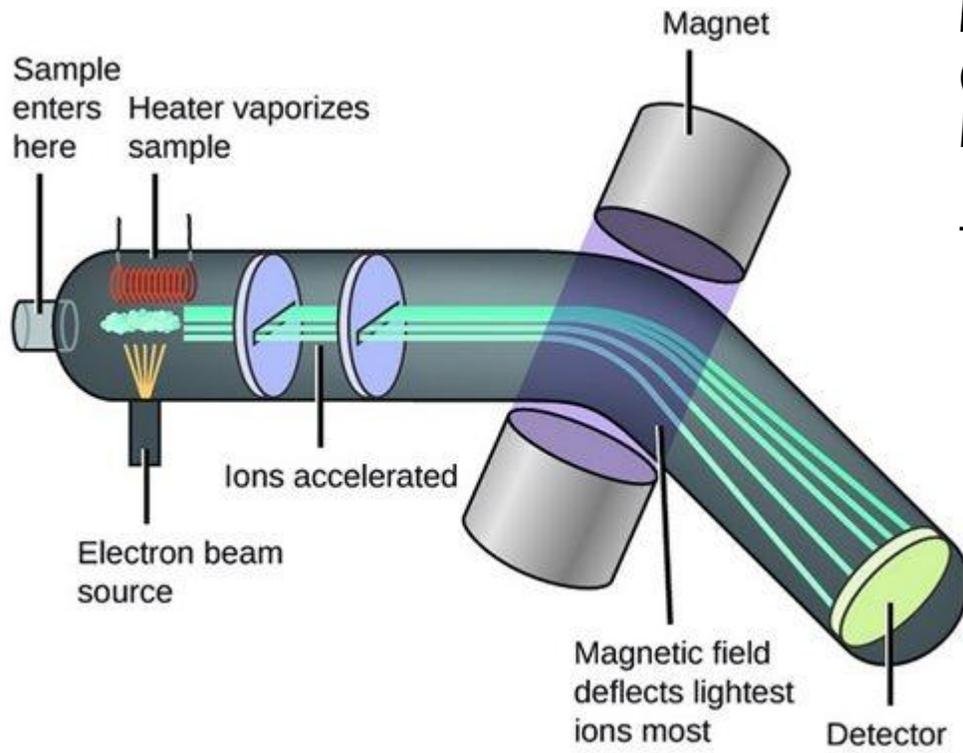


MALDI-ToF

(Matrix Assisted Laser Desorption Ionization – Time of Flight)


Tecnologia nata negli anni 80 per scopi di ricerca

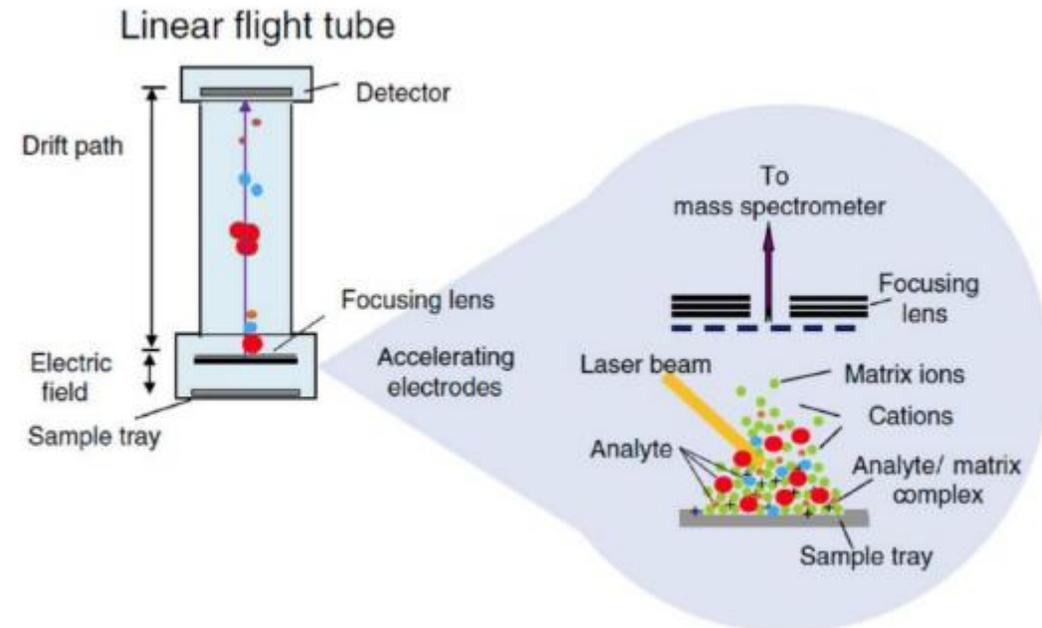

1

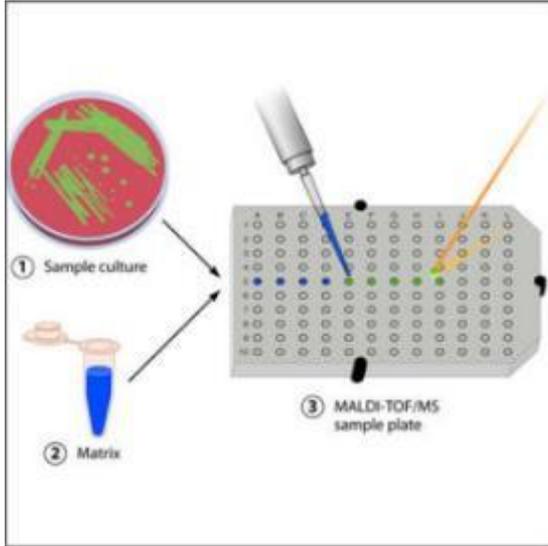


2

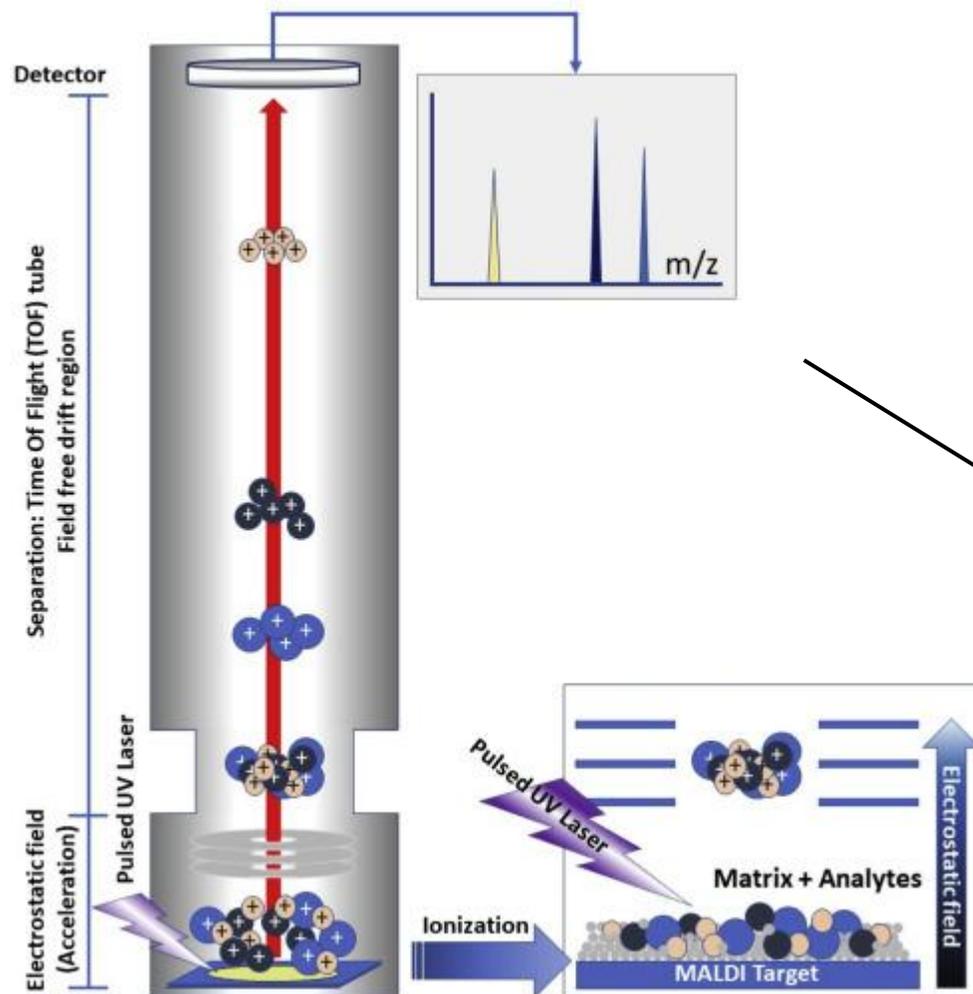

Introdotta in microbiologia dopo il 2000 da grandi aziende come Bruker e Biomerieux

3

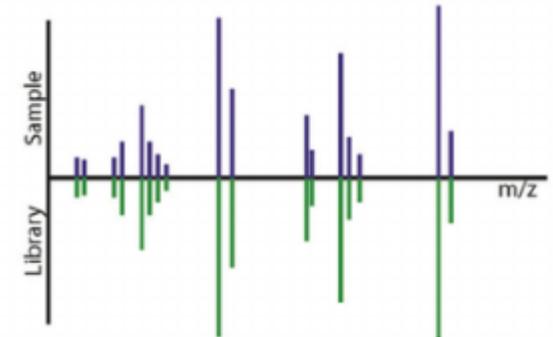

Output

Sample	Rate	Matched Pattern	Score Value
ID	1	Bacteria starin#	XXXX
	2	Bacteria starin#	XXXX
	3	Bacteria starin#	XXXX





CONTESTO DEL LABORATORIO DIAGNOSTICO MICROBIOLOGICO

IDEA



REALTA'



MICROBIAL ID SCENARIO

	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
Biochemical						
Molecular method (PCR)						
MALDI-TOF						

MICROBIAL ID SCENARIO

	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
Biochemical						
Molecular method (PCR)						
MALDI-TOF						

COSA SERVE QUINDI??

	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
Biochemical						
Molecular method (PCR)						
MALDI-TOF						
ALIFAX IDEALE						

ABBIAMO GIA' TUTTE LE SOLUZIONI?



Idea



Sviluppo

Prodotto




Fattibilità

TENTATIVO 1: GAS CROMATOGRAFIA



**Micro GC per analisi gas
prodotti dal metabolismo
microbico**

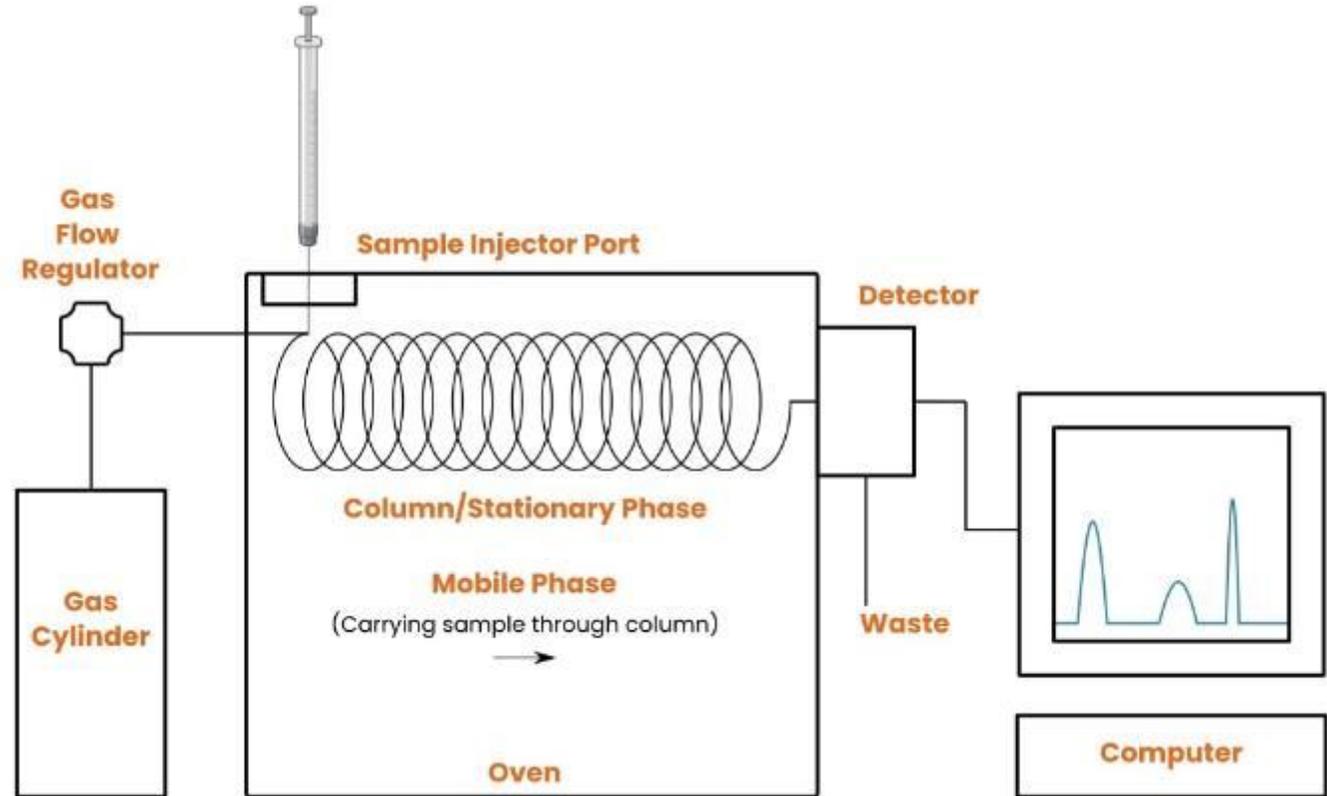


TENTATIVO 1: GAS CROMATOGRAFIA

Svantaggi

- Ridotta informazione delle componenti misurabili;
- Elevata manutenzione attrezzatura;
- Necessità di gas «carrier» costantemente disponibile (costi, reperibilità, sicurezza)
- Prelievo campione richiedeva crescita in ambiente chiuso e sigillato, diverso da routine.




	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
ALIFAX IDEALE						

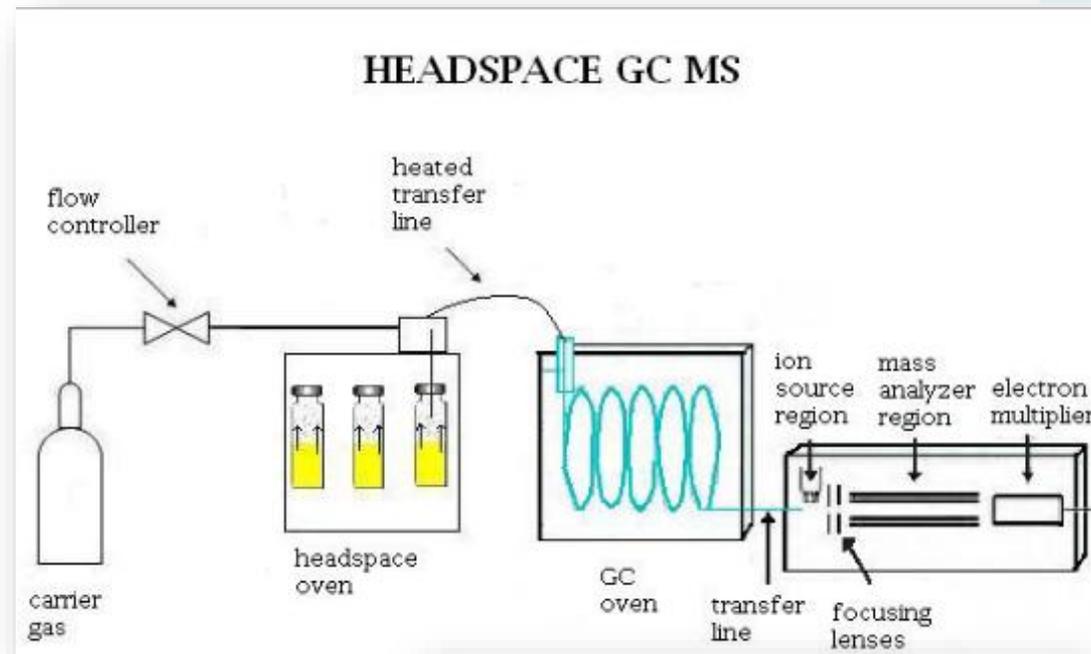

GC-MS per analisi metaboliti spazio di testa

Campionamento **SPME** (solid-phase micro extraction) da coltura liquida

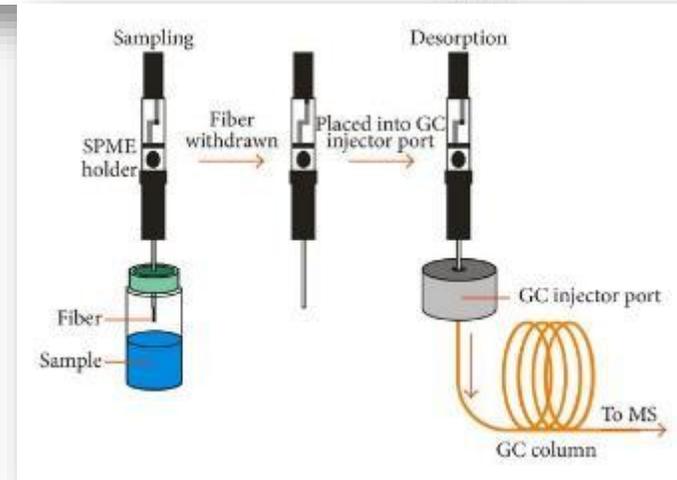


Svantaggi

- Costo attrezzatura necessaria e manutenzione;
- Utilizzo di sistema di campionamento SPME da sostituire di frequente;
- Necessità di gas «carrier» costantemente disponibile (costi, reperibilità, sicurezza);
- Prelievo campione richiedeva crescita in ambiente chiuso e sigillato, diverso da routine;
- Elevata variabilità di campionamento operatore dipendente.



	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
ALIFAX IDEALE						

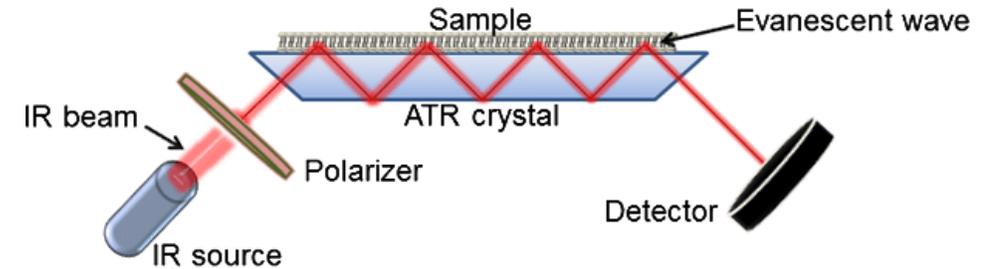

ATR: *Attenuated Total Reflection*

FTIR: *Fourier-transform infrared spectroscopy*

**Analisi di assorbimento spettroscopia
infrarossa FTIR da colonia isolata con
campionamento in ATR**


TENTATIVO 3: ATR-FTIR

Vantaggi

- ✓ Primi risultati molto promettenti fin da subito;
- ✓ Disponibilità hardware a costo contenuto e performance adeguate;
- ✓ Presenza di esperti disponibili a collaborare per attività di sviluppo;
- ✓ Campionamento estremamente robusto e indipendente da operatore;
- ✓ Assenza di consumabili, reattivi, manutenzione.



Agilent

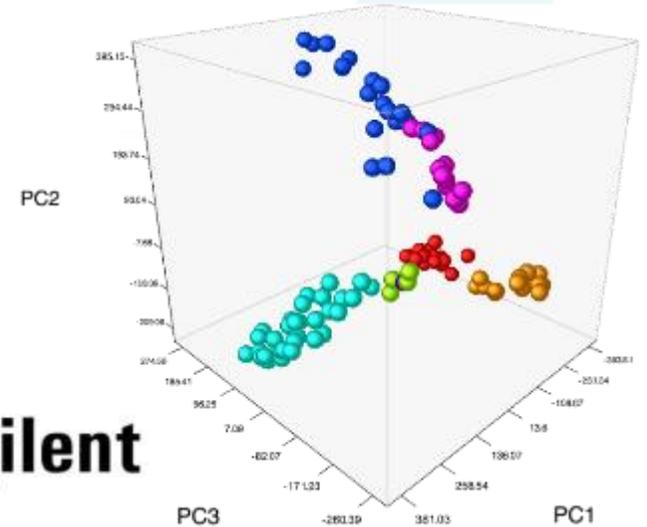


Elettra Sincrotrone Trieste

	Time to ID	Sample preparation	Costs per test	Purchase & Maintenance	ID capacity	Dimensions
ALIFAX IDEALE						



**FAIL FAST.
FAIL CHEAP.
TRY AGAIN.**

What Most People Think

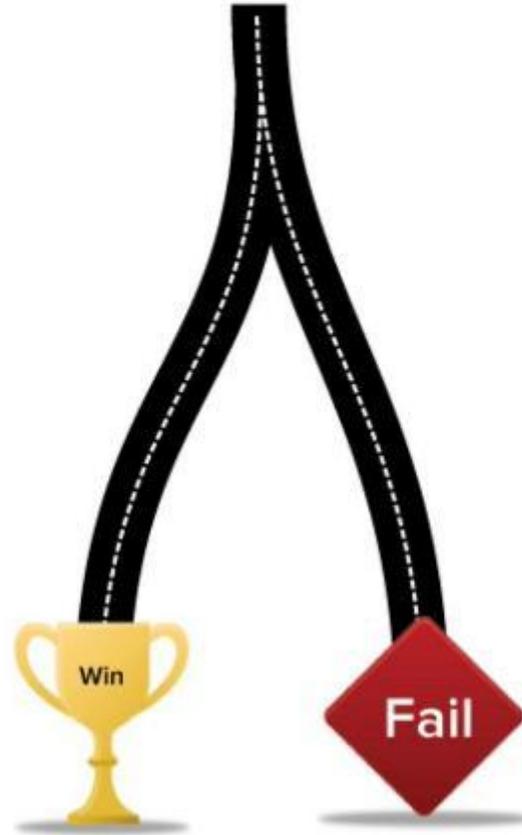


What Successful People Know



@douglaskarr


I-dOne

Sistema di identificazione microbica basato sull'interpretazione di spettri di assorbimento infrarosso tramite ATR-FTIR

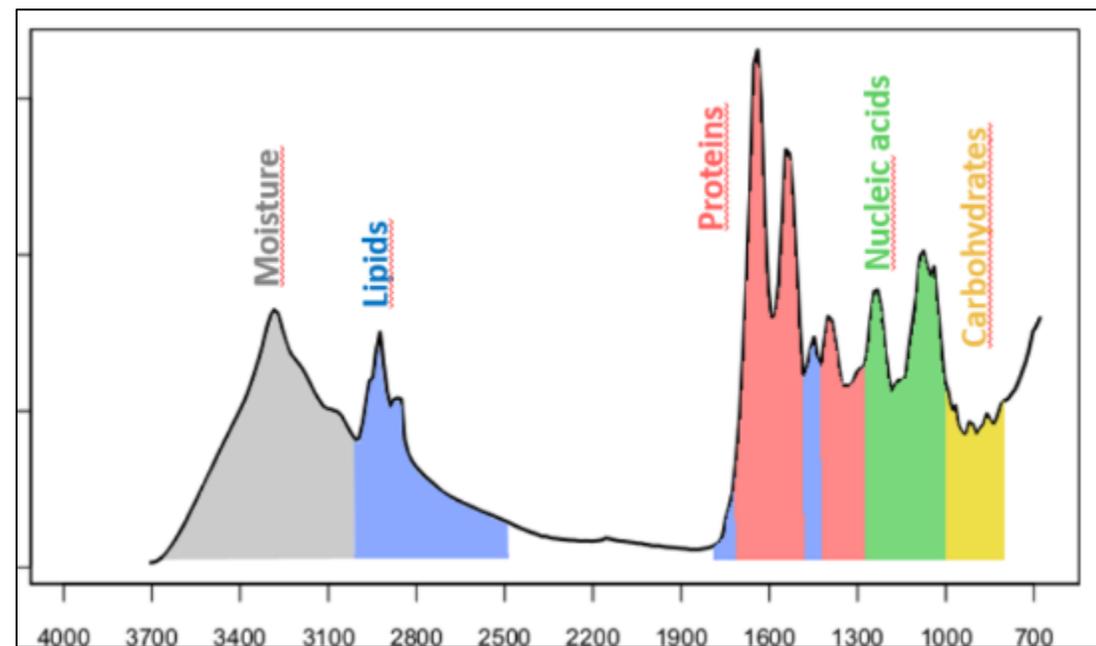

TECNOLOGIA_1

RADIAZIONE INFRAROSSA

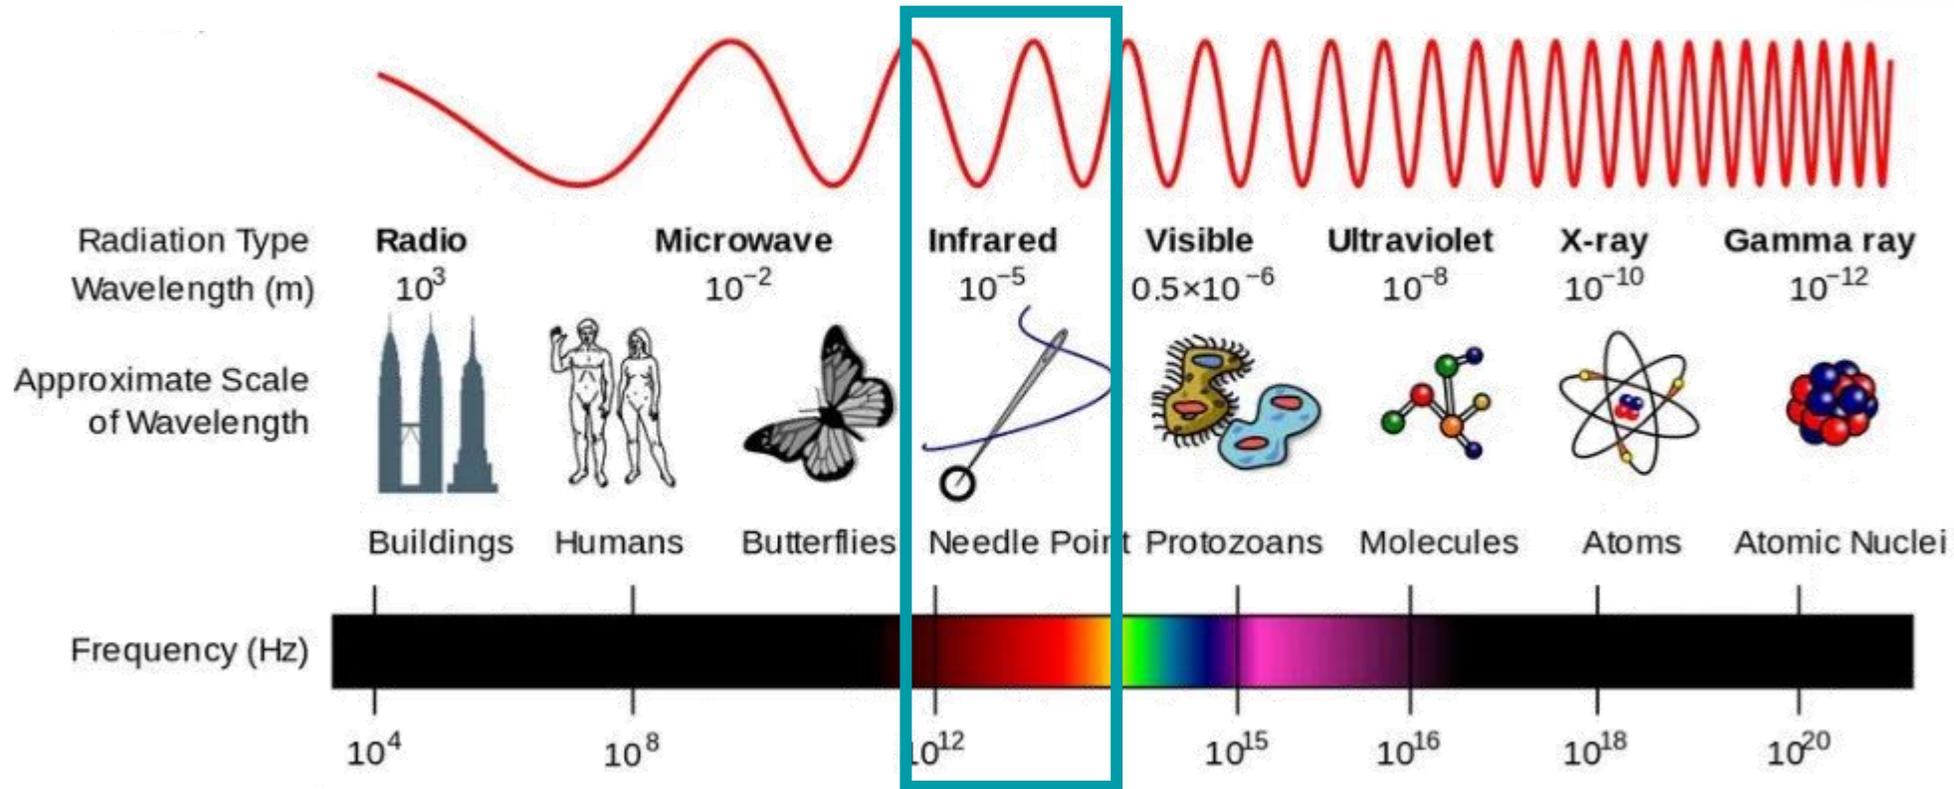


IR RANGE:
1-10 μm


TECNOLOGIA_2

ASSORBIMENTO INFRAROSSO


Bonds absorb InfraRed energy by increasing their vibrational state in relation to their specific molecular structure.




symmetric stretching



asymmetric stretching




scissoring




rocking

The InfraRed spectrum of a bacterial sample is considered to be its most characteristic physical property and serves as its molecular fingerprint for definitive identification.

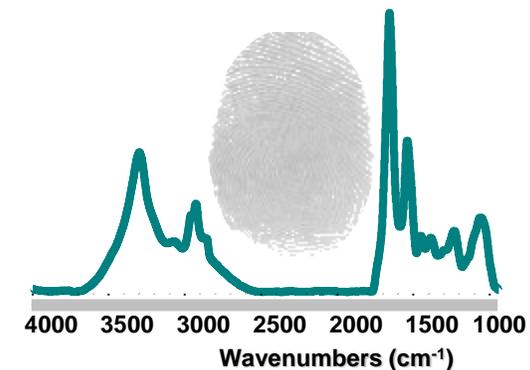

The ATR-FTIR Approach (ATR: Attenuated Total Reflection)

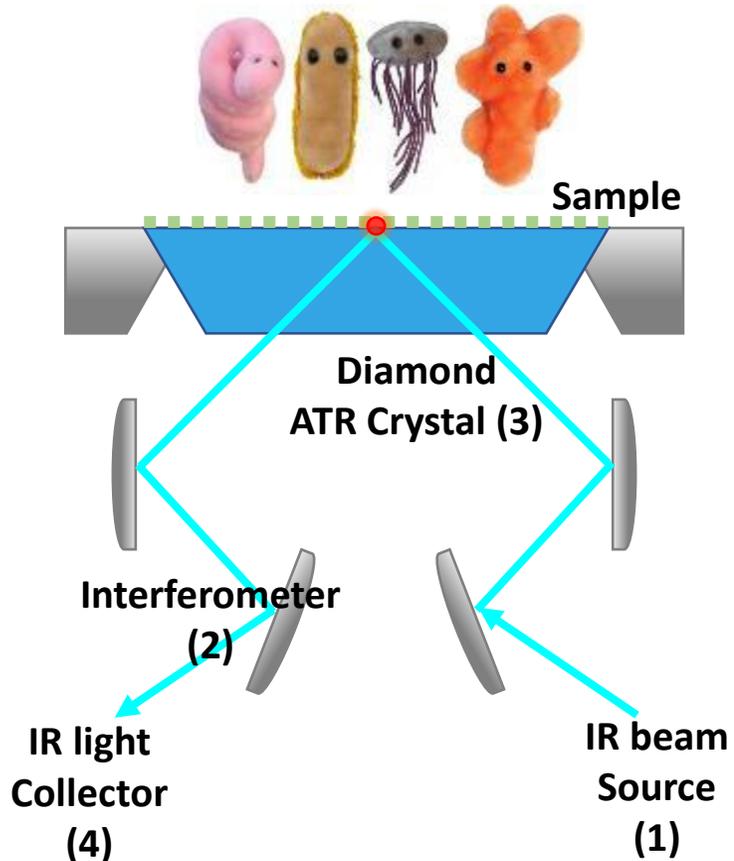

We illuminate the sample from the bottom of a reading crystal on which the sample is placed. At the interface between crystal and sample the absorption of the IR light occur by the sample. **The capacity of the incident light to penetrate the sample is called evanescent wave.** The residual beam is thus collected from the detector. The difference between the absorption profile with and without the sample makes the absorption spectrum.

Advantage: the penetration depth of the IR light is independent from the sample. IR light is able to penetrate the sample for hundreds of nanometers. Thus:

- Intensity does not depend on sample concentration
- A very small amount of sample is enough

ATTIVITA' TECNICHE DI SVILUPPO



Raccolta ceppi microbici



ID di riferimento






Crescita in diverse condizioni



Misura spettri IR




Creazione database di riferimento con oltre 20.000 spettri (in crescita costante)

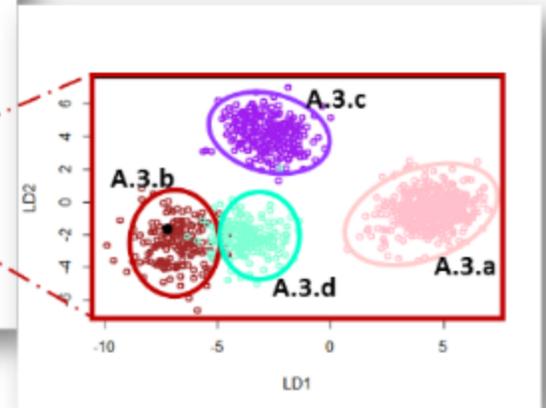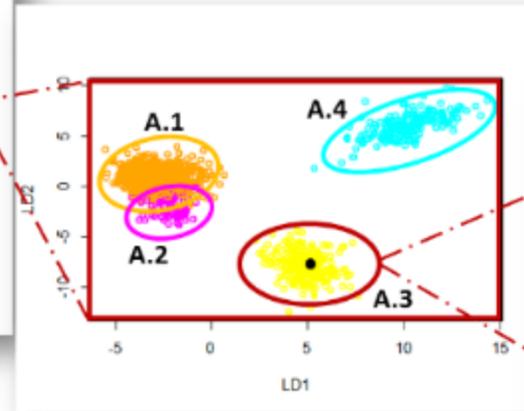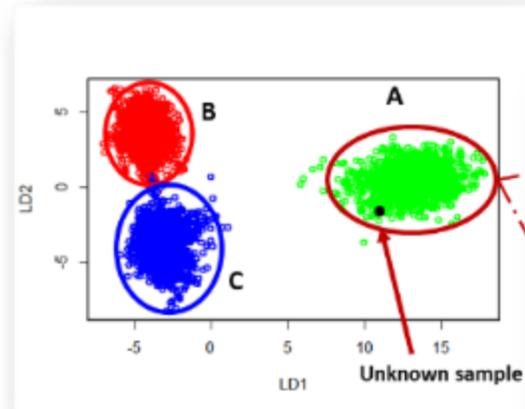



Sviluppo algoritmo di identificazione

I-DONE: STORIA DI UN PROGETTO

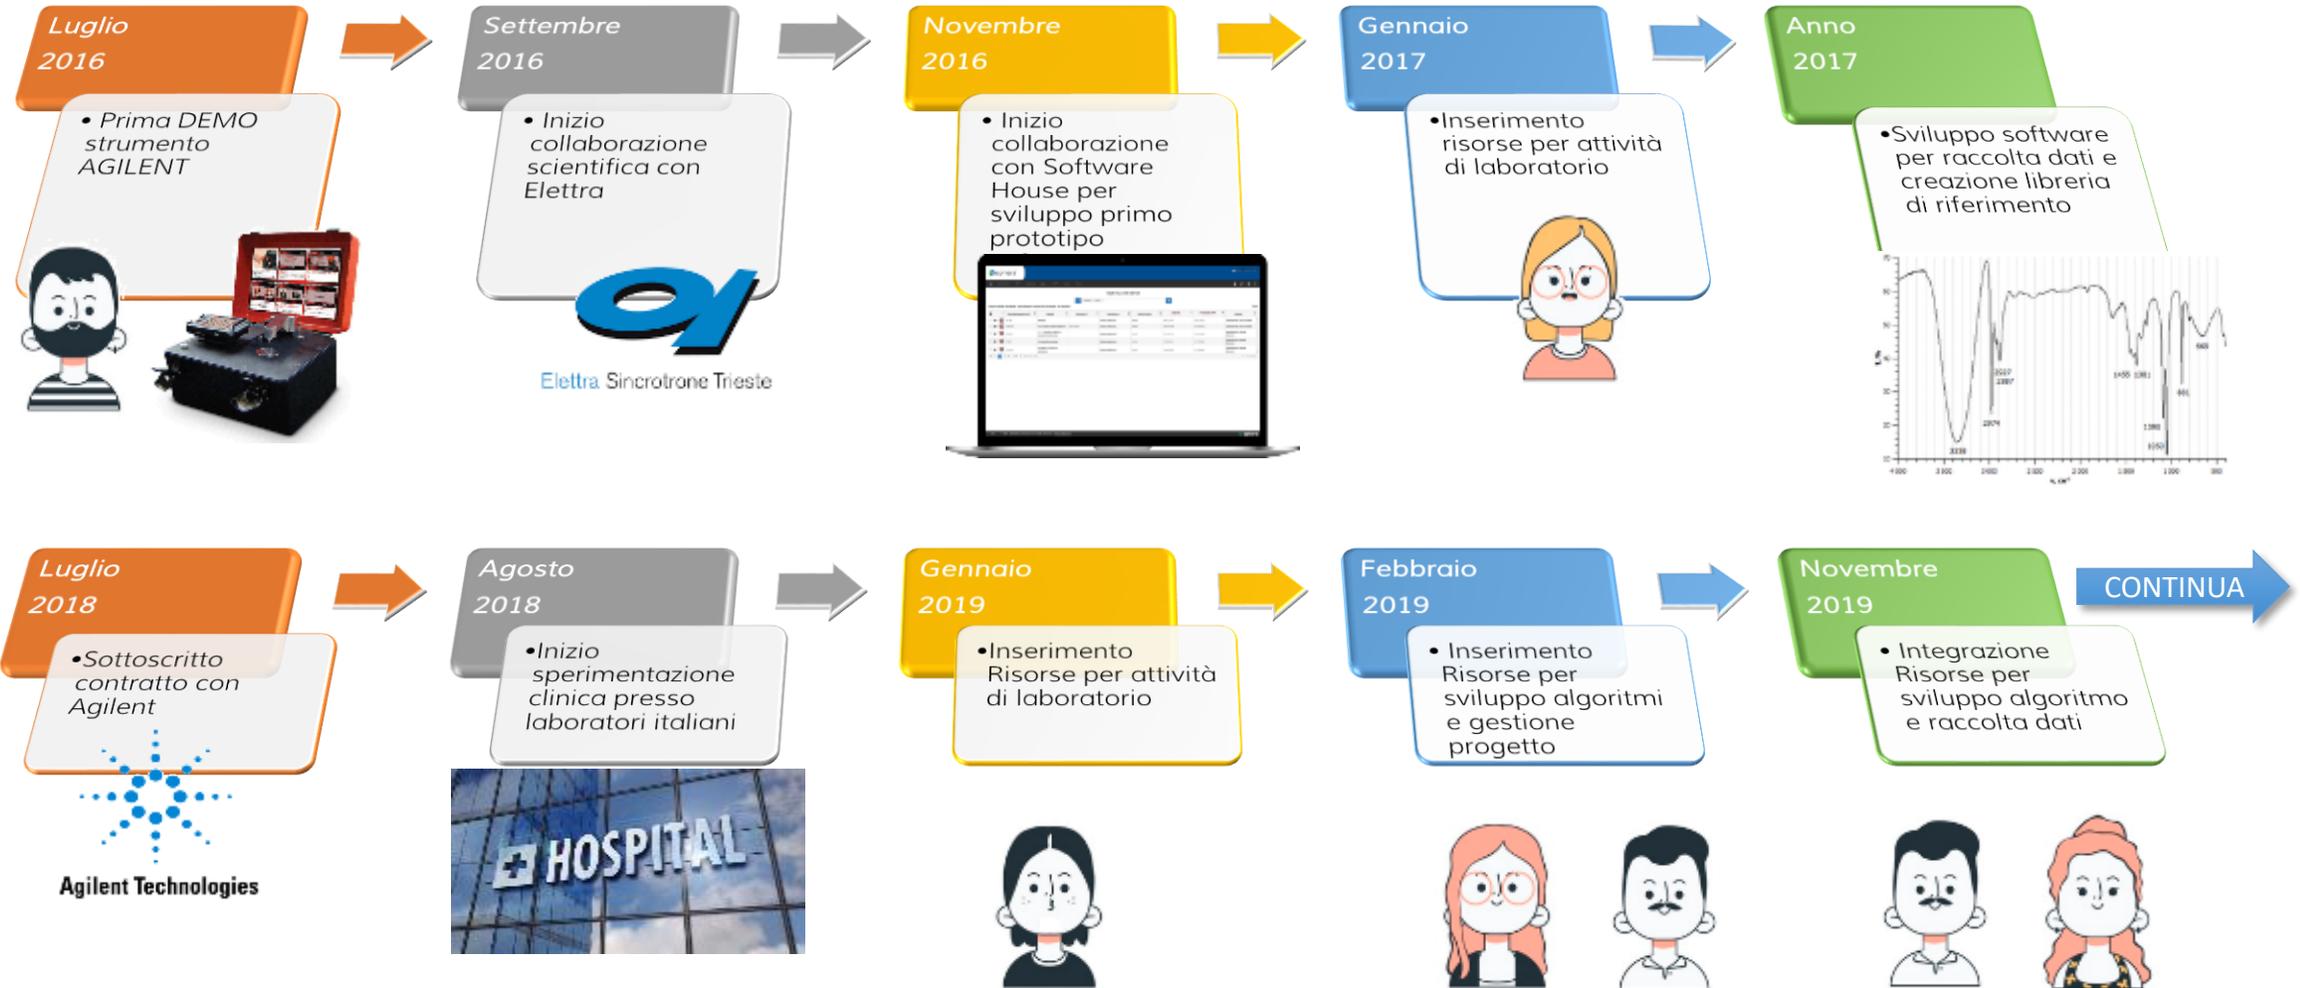


COME ARRIVARE A UN PRODOTTO?

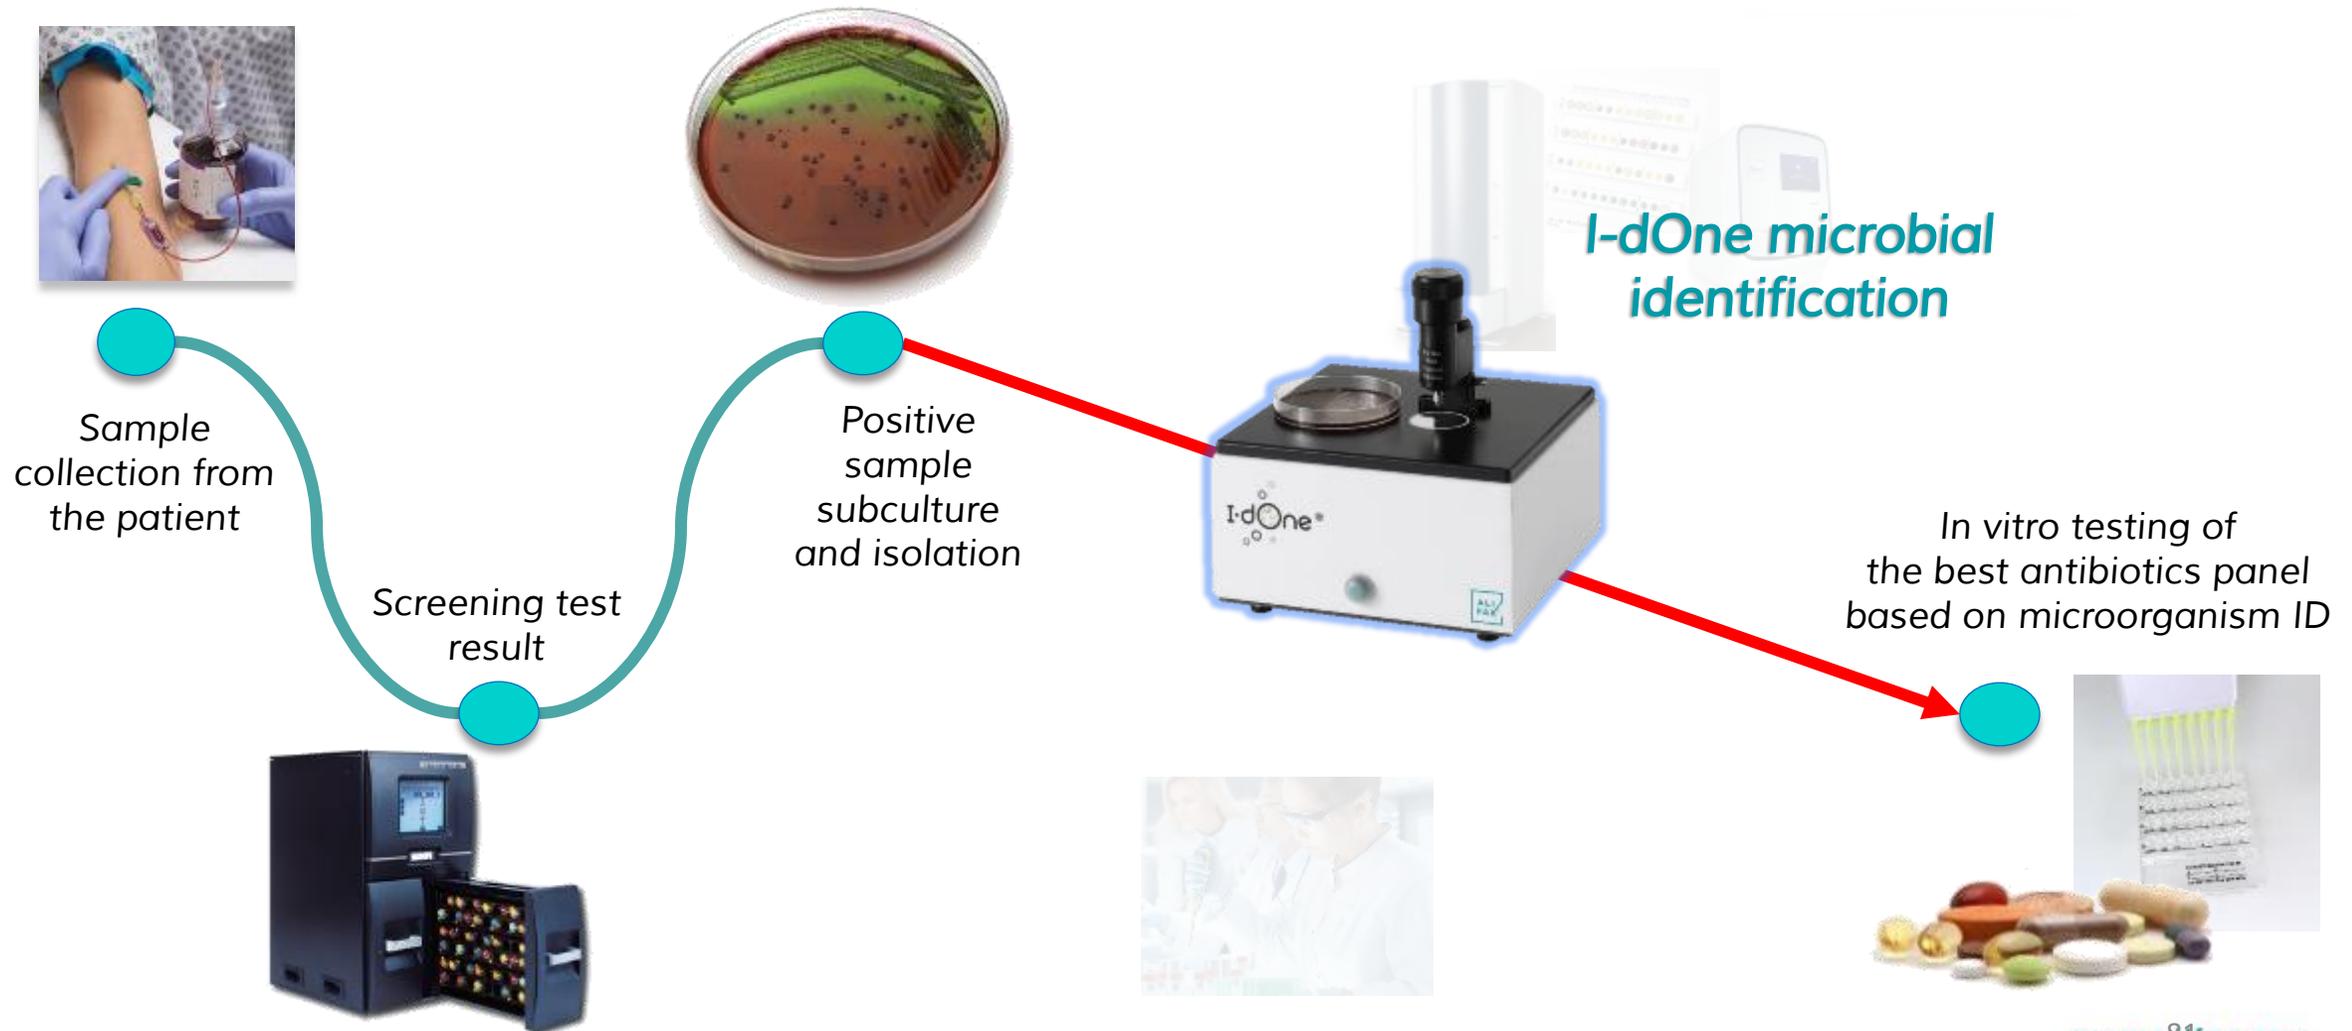

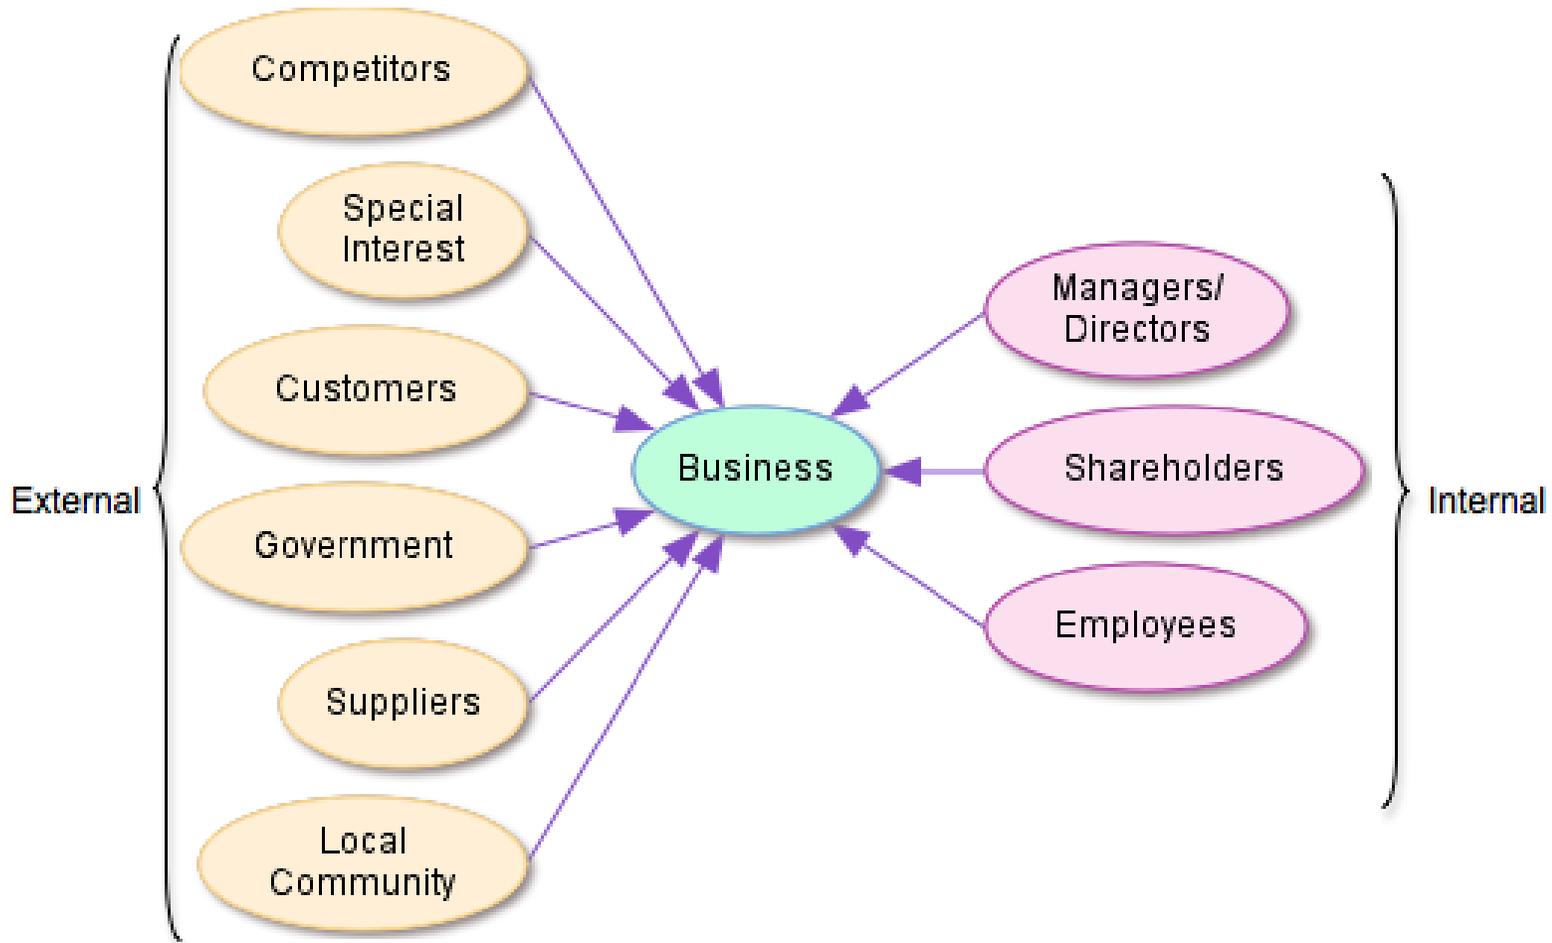

Stakeholder (portatore di interesse) è genericamente qualsiasi soggetto o gruppo coinvolto in una qualsiasi iniziativa economica, una società o altro progetto, e in generale con interessi legati all'esecuzione o dall'andamento dell'iniziativa stessa.

STAKEHOLDER DI PROGETTO

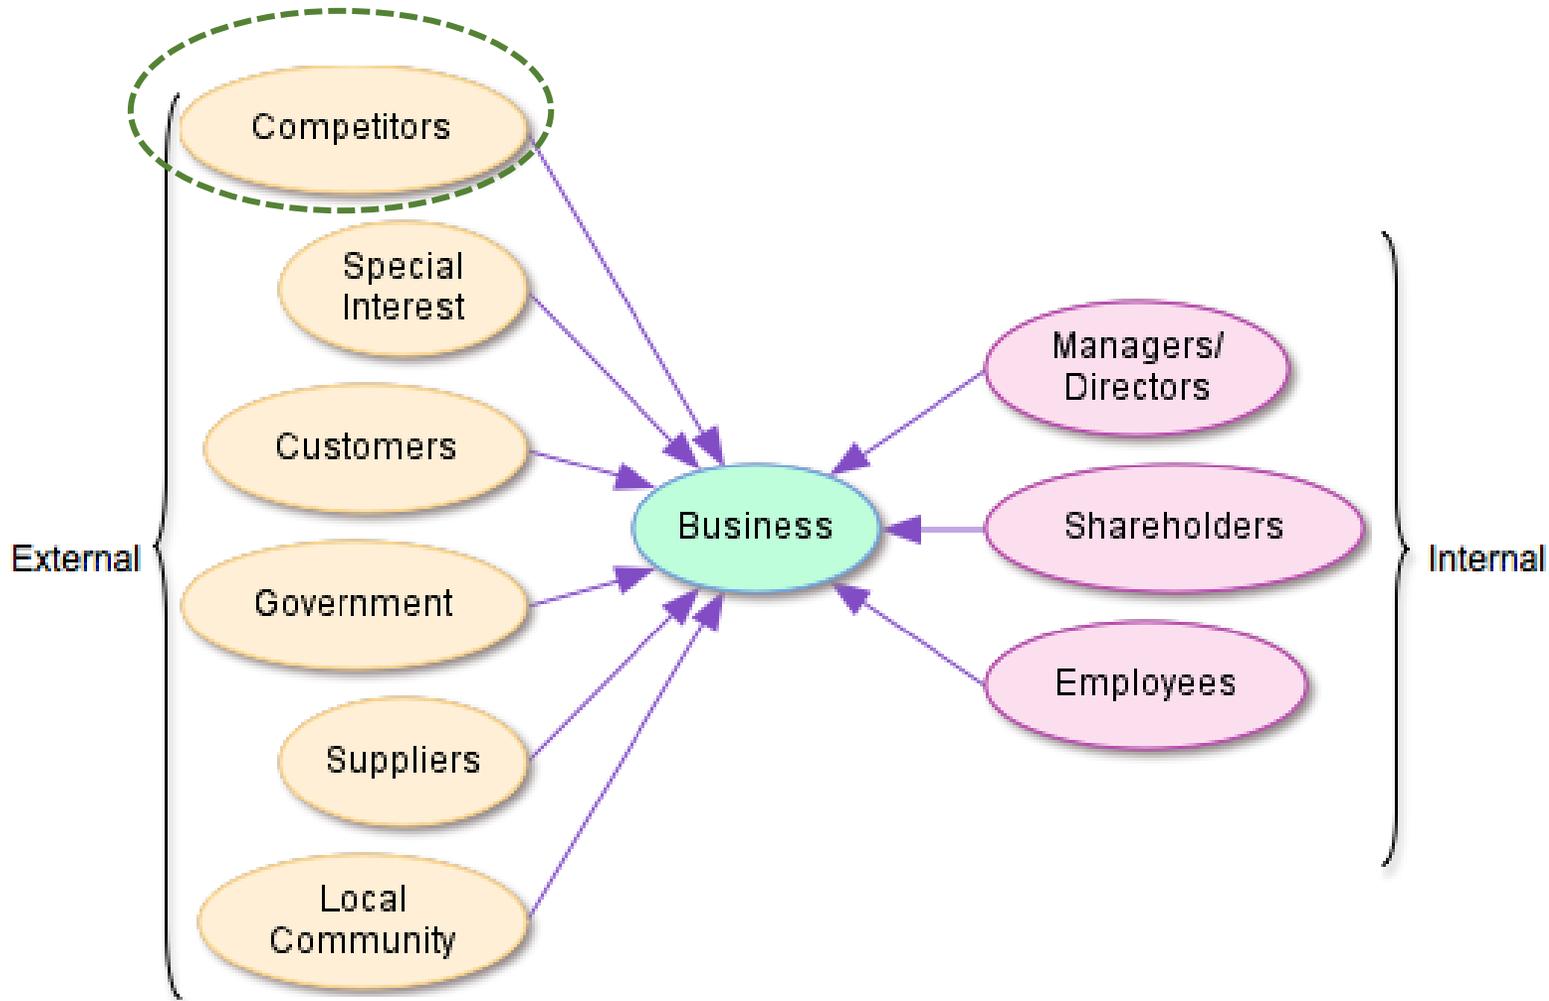



TUTELARSI DAI COMPETITORS

INSIDE INNOVATION

<https://www.epo.org/searching-for-patents.html>



Home > Searching for patents


Searching for patents


Print Share

<https://patents.google.com/>




Verificare lo spazio brevettuale disponibile per sviluppare la propria idea in area non coperte da competitors e tutelare le proprie applicazioni tramite la scrittura di brevetti

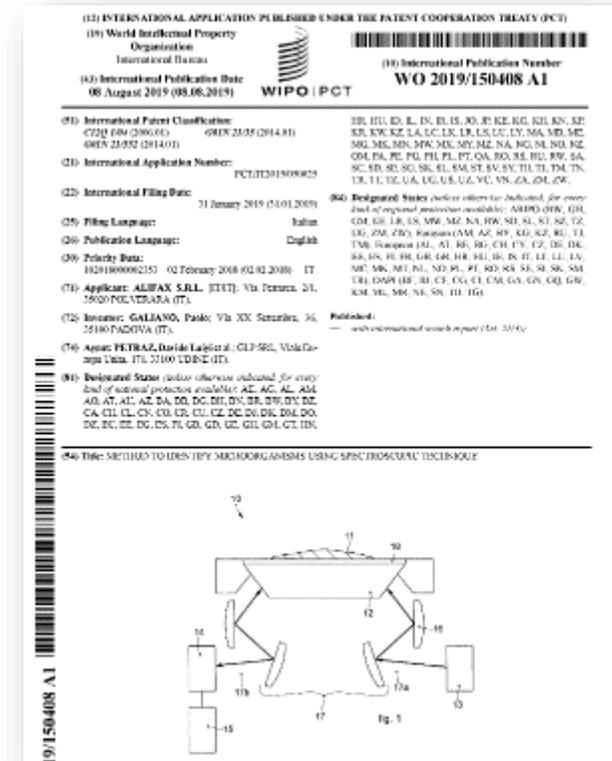


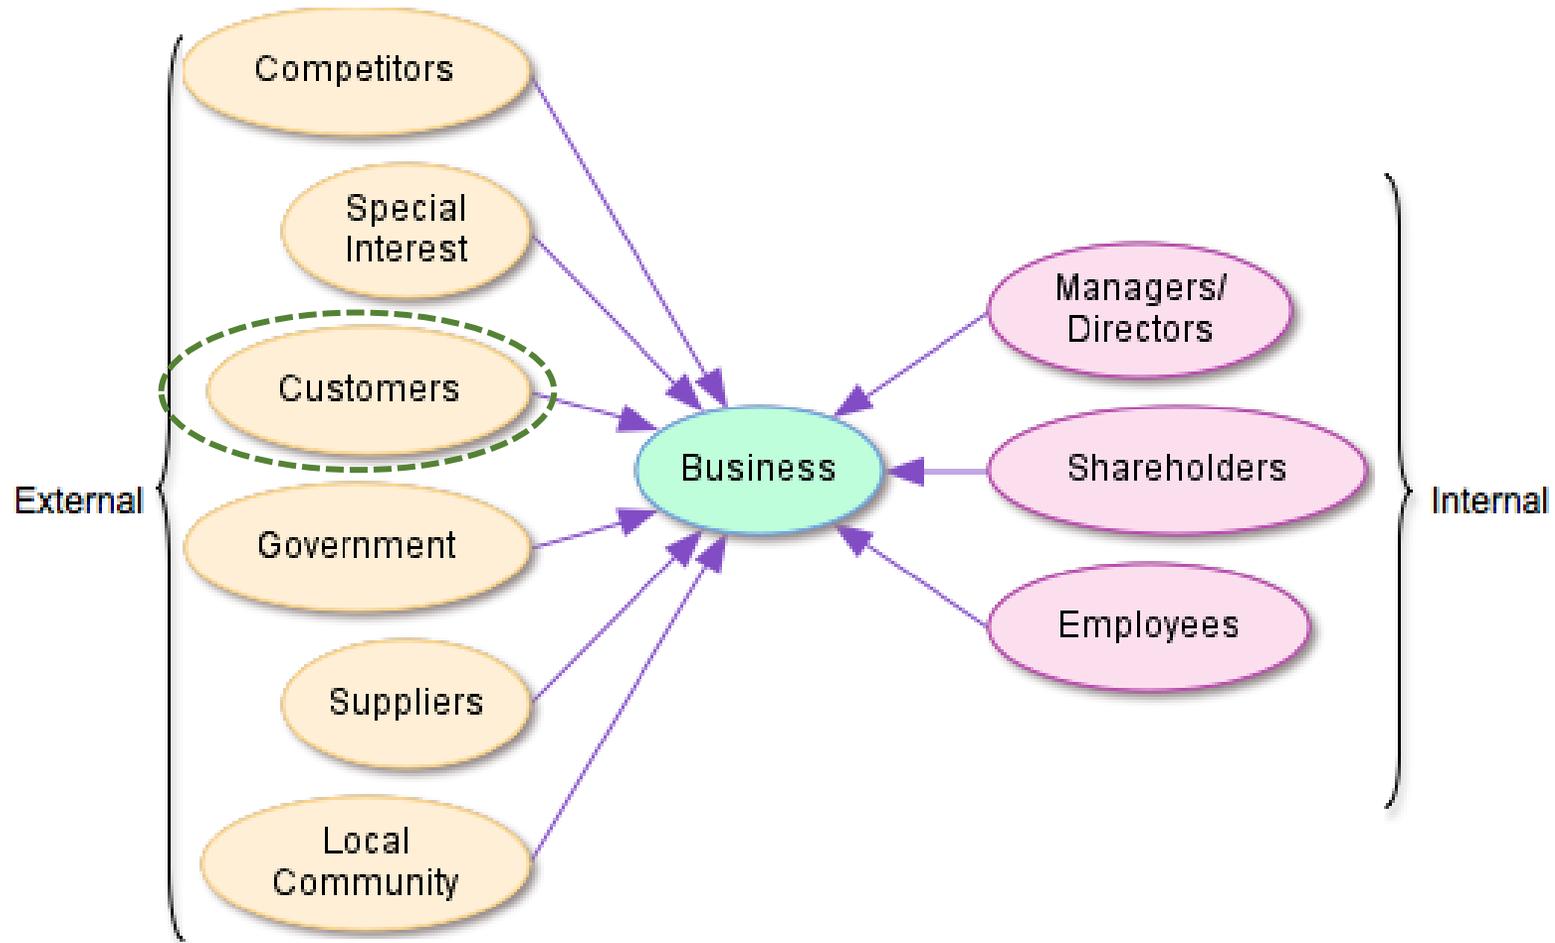

IDENTIFICARE I CUSTOMER (USER) NEEDS

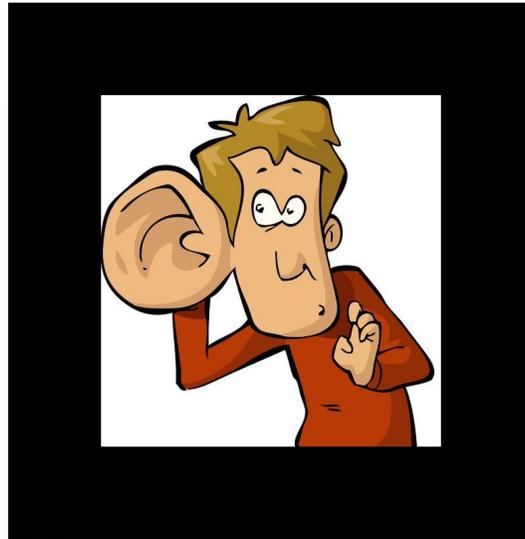

UNDERCOVER BOSS

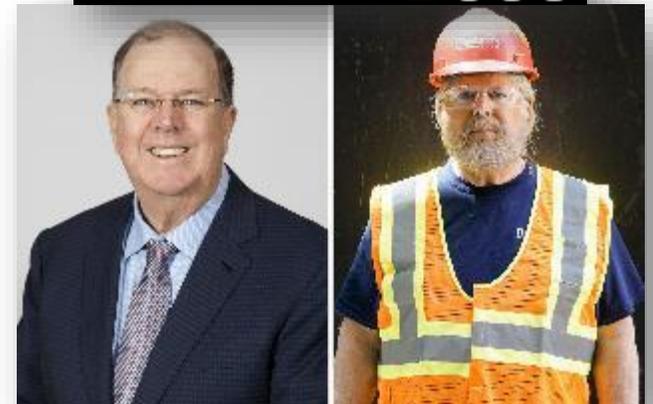



Chi sono gli user???





Chi sono gli user????




- **Addetto Produzione**
- **Magazzino e Logistica (movimentazione, stoccaggio)**
- **Commerciale (promozione, impatto emotivo prodotto)**
- **Installatore (facile, veloce, completo)**
- **Utilizzatore di laboratorio (usabilità)**
- **Direttore del laboratorio (vantaggio)**
- **Assistenza Tecnica (accessibile, semplice)**



Chi sono gli user????




- Addetto Produzione
- Magazzino e Logistica (movimentazione, stoccaggio)
- Commerciale (promozione, impatto emotivo prodotto)
- Installatore (facile, veloce, completo)
- **Utilizzatore di laboratorio (USABILITA')**
- Direttore del laboratorio (vantaggio)
- Assistenza Tecnica (accessibile, semplice)

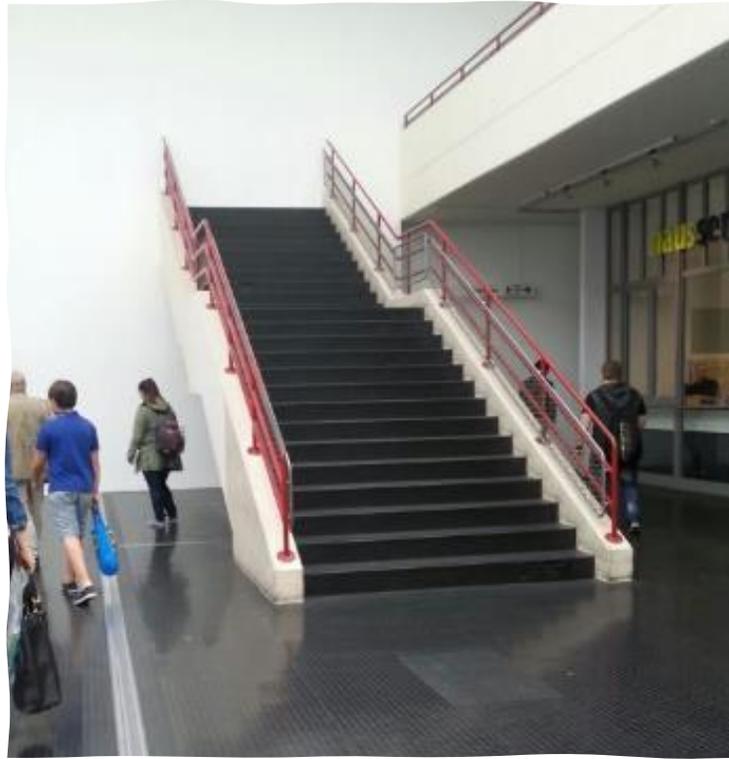

USABILITA' COME FUNZIONE



USABILITA' COME RIDUZIONE DI ERRORI

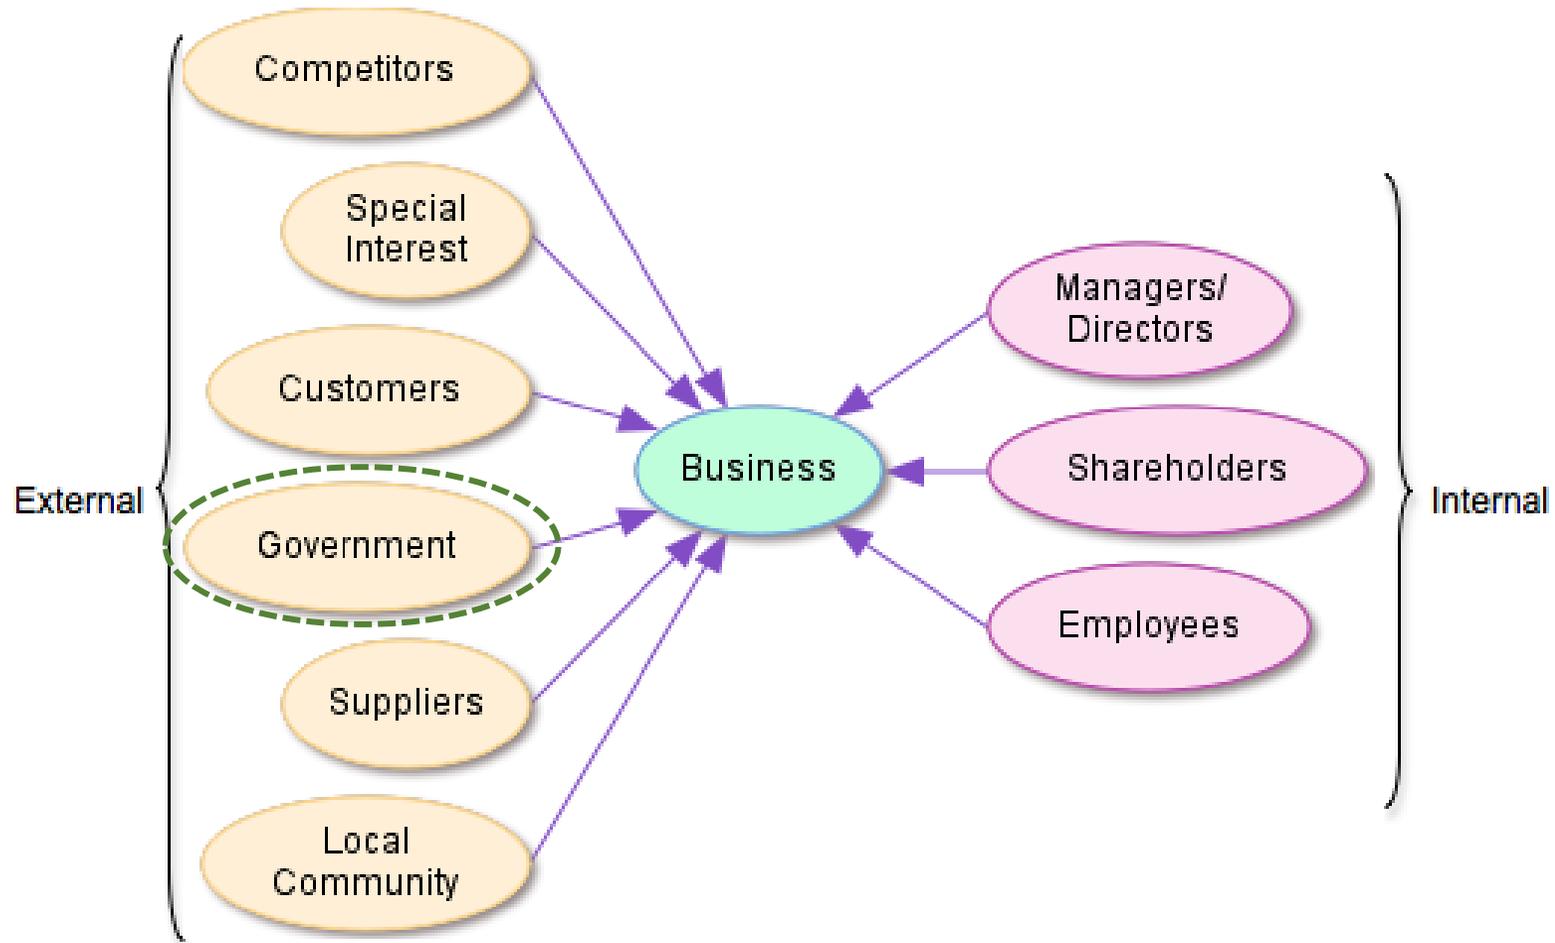

IVDR – REG EU 746/2017



Regolamenta e guida nello sviluppo di un dispositivo IVD:

- Definizione dell'Intended Use del dispositivo
- Assegnazione della classe di rischio del dispositivo
- Rispetto dei requisiti minimi di Sicurezza e Performance
- Esecuzione di prove di verifica e validazioni cliniche



GENERAL SAFETY AND PERFORMANCE REQUIREMENTS

INSIDE INNOVATION

CHAPTER I, GENERAL REQUIREMENTS

1. Devices shall achieve the performance intended by their manufacturer and shall be designed and manufactured in such a way that, during normal conditions of use, they are suitable for their intended purpose. They shall be safe and effective and shall not compromise the clinical condition or the safety of patients, or the safety and health of users or, where applicable, other persons, provided that any risks which may be associated with their use constitute acceptable risks when weighed against the benefits to the patient and are compatible with a high level of protection of health and safety, taking into account the generally acknowledged state of the art.

GENERAL SAFETY AND PERFORMANCE REQUIREMENTS

CHAPTER I, GENERAL	CHAPTER II, REQUIREMENTS REGARDING DESIGN AND MANUFACTURE	
<p>1. Devices shall achieve the safety and performance intended by their manufacturer, designed and manufactured in accordance with the requirements during normal conditions of use, and shall perform their intended purpose. They shall be safe, effective and shall not cause any harm to the user, condition or the safety of the user, or the health of users or, where applicable, the health of animals, provided that any risks which are acceptable against the benefits to the user, and which are taken into account with a high level of protection, taking into account the general principles of the art.</p>	<p>10. Chemical, physical and biological properties</p>	
	<p>10.1. Devices shall be designed and manufactured in such a way as to ensure that the characteristics and performance requirements referred to in Chapter I are fulfilled. Particular attention shall be paid to:</p>	
	<p>(a) the choice of materials and substances used, particularly as regards toxicity and, where relevant, flammability;</p>	
	<p>(b) the compatibility between the materials and substances used and biological tissues, cells and body fluids, taking account of the intended purpose of the device and, where relevant, absorption, distribution, metabolism and excretion;</p>	
	<p>(c) the compatibility between the different parts of a device which consists of more than one implantable part;</p>	


GENERAL SAFETY AND PERFORMANCE REQUIREMENTS

<p>CHAPTER I, GENERAL</p>	<p>CHAPTER II, REQUIREMENTS REGARDING</p>	<p>11. Infection and microbial contamination</p>
<p>1. Devices shall achieve the intended purpose of their intended use during normal conditions of use and shall not compromise the safety or health of users or, where applicable, the safety of their use constitute acceptable risks against the benefits to be derived from their use with a high level of protection taking into account the general principles of the art.</p>	<p>10. Chemical, physical and biological properties</p>	
	<p>10.1. Devices shall be designed and manufactured in such a way as to ensure that the characteristics and performance requirements referred to in 10.1 are fulfilled. Particular attention shall be paid to:</p>	<p>11.1. Devices and their manufacturing processes shall be designed in such a way as to eliminate or to reduce as far as possible the risk of infection to patients, users and, where applicable, other persons. The design shall:</p> <ul style="list-style-type: none"> (a) reduce as far as possible and appropriate the risks from unintended cuts and pricks, such as needle stick injuries, (b) allow easy and safe handling, (c) reduce as far as possible any microbial leakage from the device and/or microbial exposure during use, and (d) prevent microbial contamination of the device or its content such as specimens or fluids.
	<p>(a) the choice of materials and substances used, particularly as regards toxicity and, where applicable, flammability;</p>	<p>11.2. Where necessary devices shall be designed to facilitate their safe cleaning, disinfection, and/or re-sterilisation.</p>
	<p>(b) the compatibility between the materials used and biological tissues, cells and body fluids, taking account of the intended use of the device and, where relevant, absorption, distribution, metabolism and excretion;</p>	
	<p>(c) the compatibility between the different parts of a device which consists of more than one implantable part;</p>	


GENERAL SAFETY AND PERFORMANCE REQUIREMENTS

CHAPTER I, GENERAL	CHAPTER II, REQUIREMENTS REGARDING	11. Infection and microbial c	17. Electronic programmable systems — devices that incorporate electronic programmable systems and software that are devices in themselves
<p>1. Devices shall achieve the safety and performance intended by their manufacturer, designed and manufactured in accordance with the requirements during normal conditions of use, and shall perform their intended purpose. The device shall be effective and shall not create any hazard or condition or the safety or health of users or, where applicable, the safety of the environment, provided that any risks which are inherent in their use constitute an acceptable level of risk against the benefits to be derived from their use with a high level of protection, taking into account the general principles of the art.</p>	<p>10. Chemical, physical and biological properties</p> <p>10.1. Devices shall be designed and manufactured in such a way as to ensure that the characteristics and performance requirements referred to in 10.1 are fulfilled. Particular attention shall be paid to:</p> <ul style="list-style-type: none"> (a) the choice of materials and substances used, particularly as regards toxicity and, where applicable, flammability; (b) the compatibility between the materials and substances used and biological tissues, cells, body fluids, taking account of the intended use of the device and, where relevant, absorption, distribution, metabolism and excretion; (c) the compatibility between the different parts of a device which consists of more than one implantable part; 	<p>11.1. Devices and their manufacturer shall be designed in such a way as to reduce as far as possible the risks to patients, users and, where applicable, the environment. The design shall:</p> <ul style="list-style-type: none"> (a) reduce as far as possible all risks from unintended cuts and needle stick injuries, (b) allow easy and safe handling, (c) reduce as far as possible all risks from the device and/or microbial contamination, use, and (d) prevent microbial contamination of the device or its content such as specimens or fluids. <p>11.2. Where necessary devices shall be designed to facilitate their safe cleaning, disinfection, and/or re-sterilisation.</p>	<p>17.1. Devices that incorporate electronic programmable systems, including software, or software that are devices in themselves, shall be designed to ensure repeatability, <u>reliability</u> and performance in line with their intended use. In the event of a single fault condition, appropriate means shall be adopted to eliminate or reduce as far as possible consequent risks or impairment of performance.</p>

DAI REQUISITI AL PRODOTTO

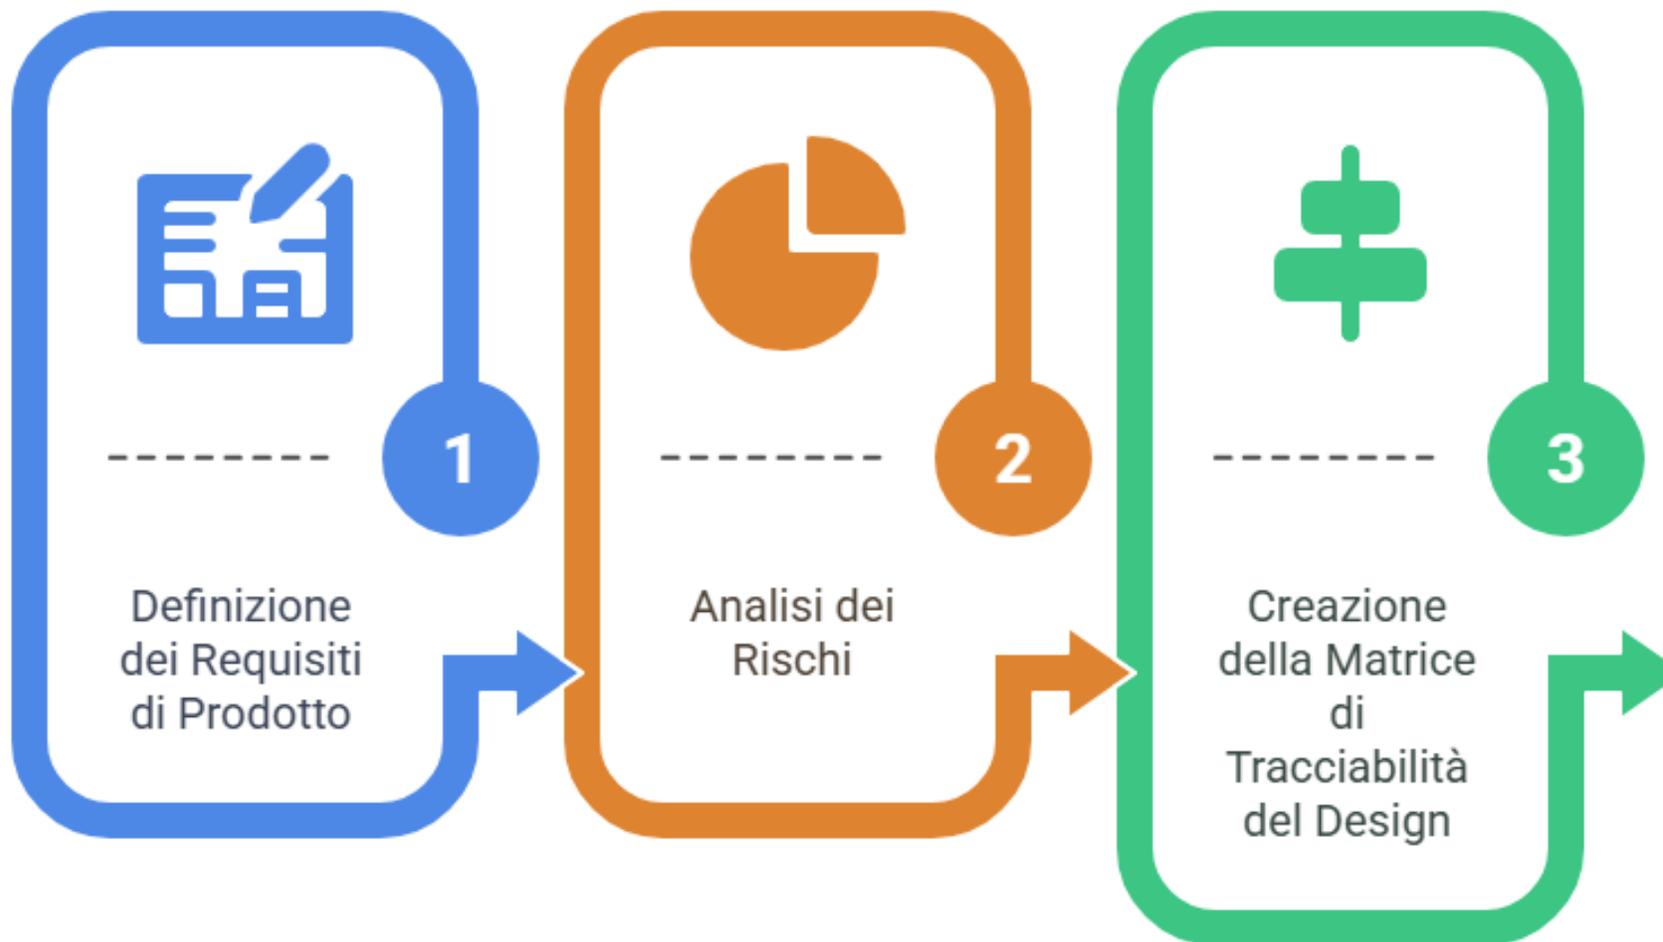


Fondamenti Essenziali per la Progettazione di Dispositivi Diagnostici


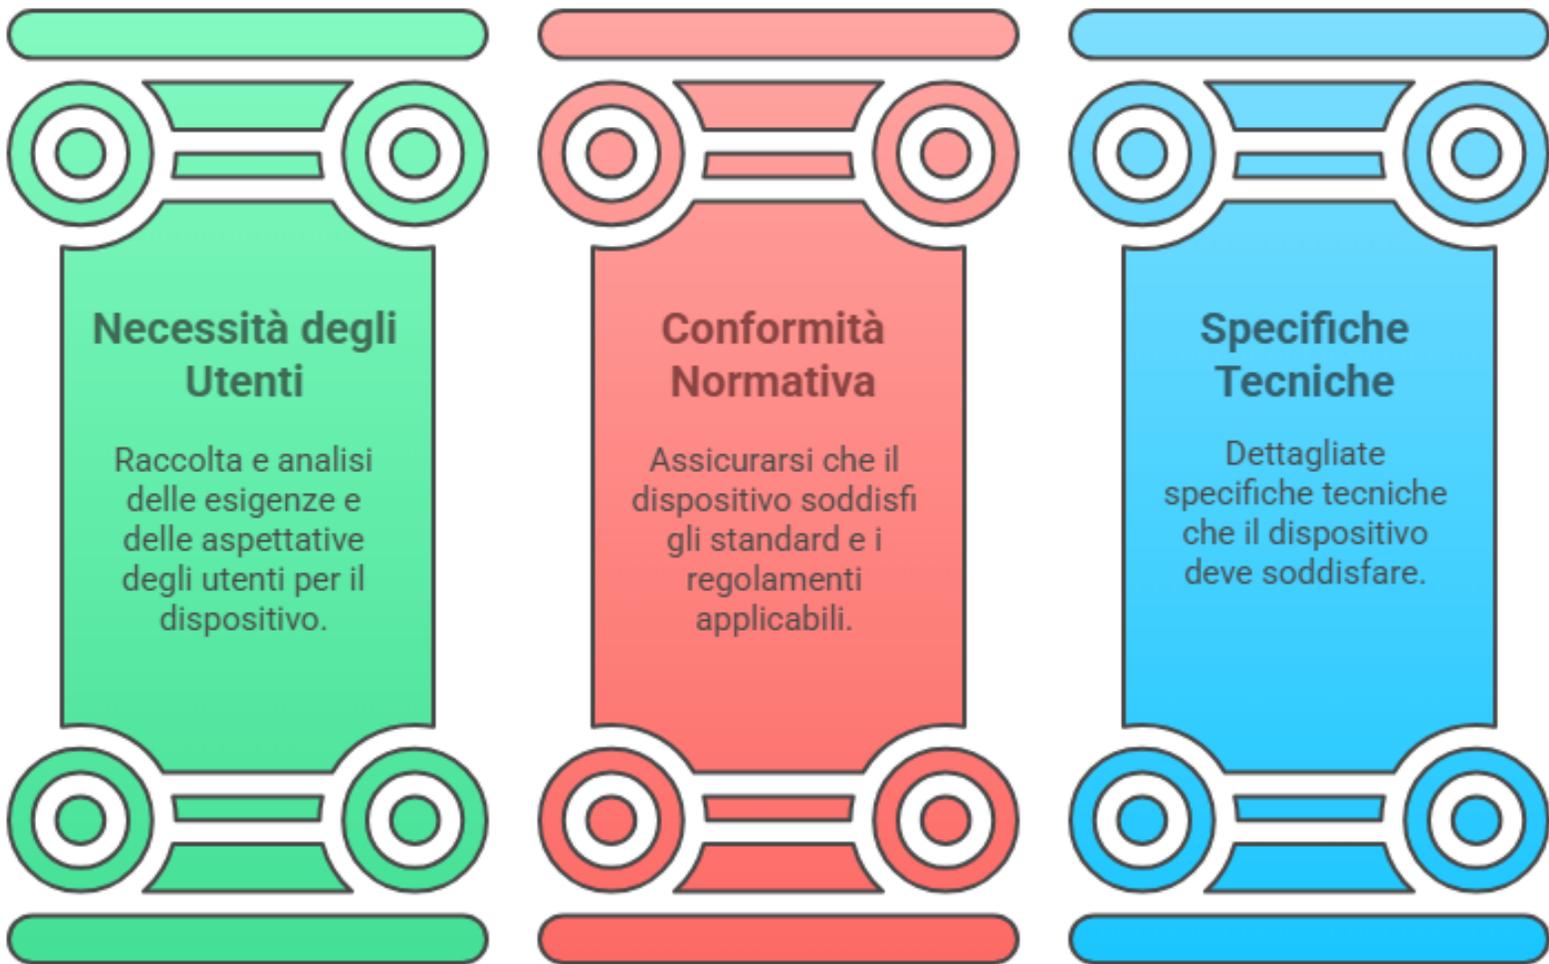


Gestione dei Rischi nel Design dei Dispositivi Diagnostici




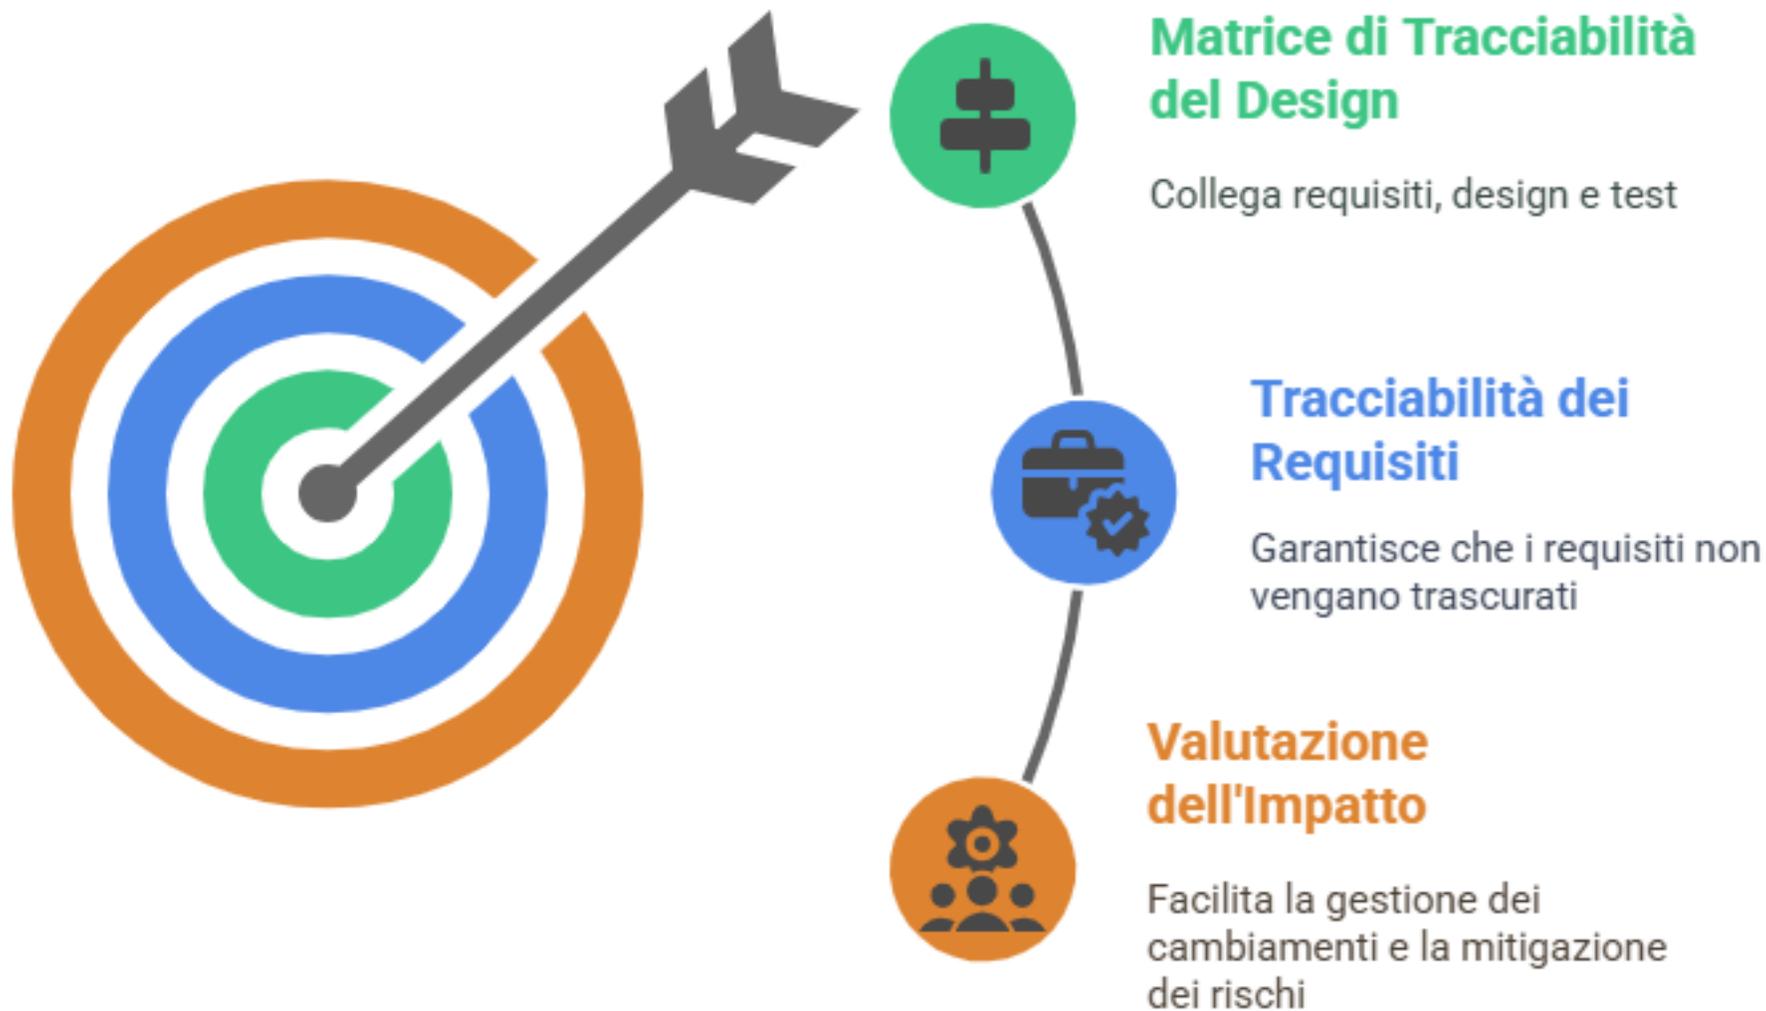

User needs
 Stakeholder needs
 Analisi dei rischi
 Requisiti Normativi

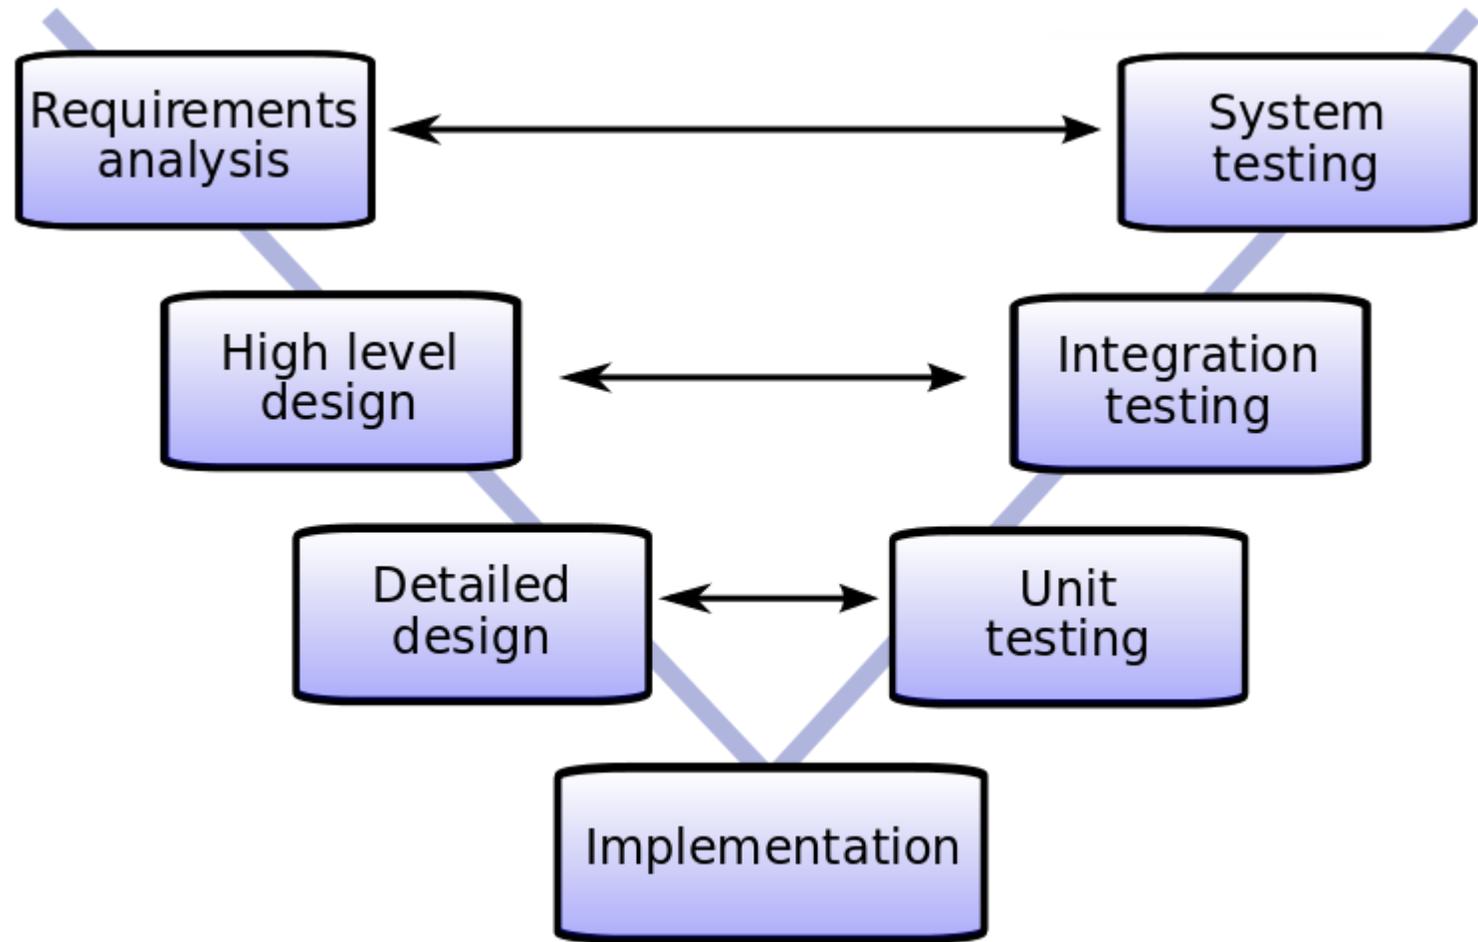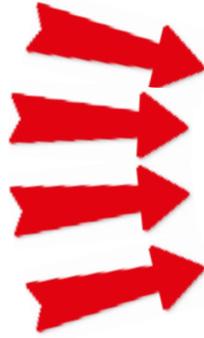

Processo di Design di un Dispositivo Diagnostico

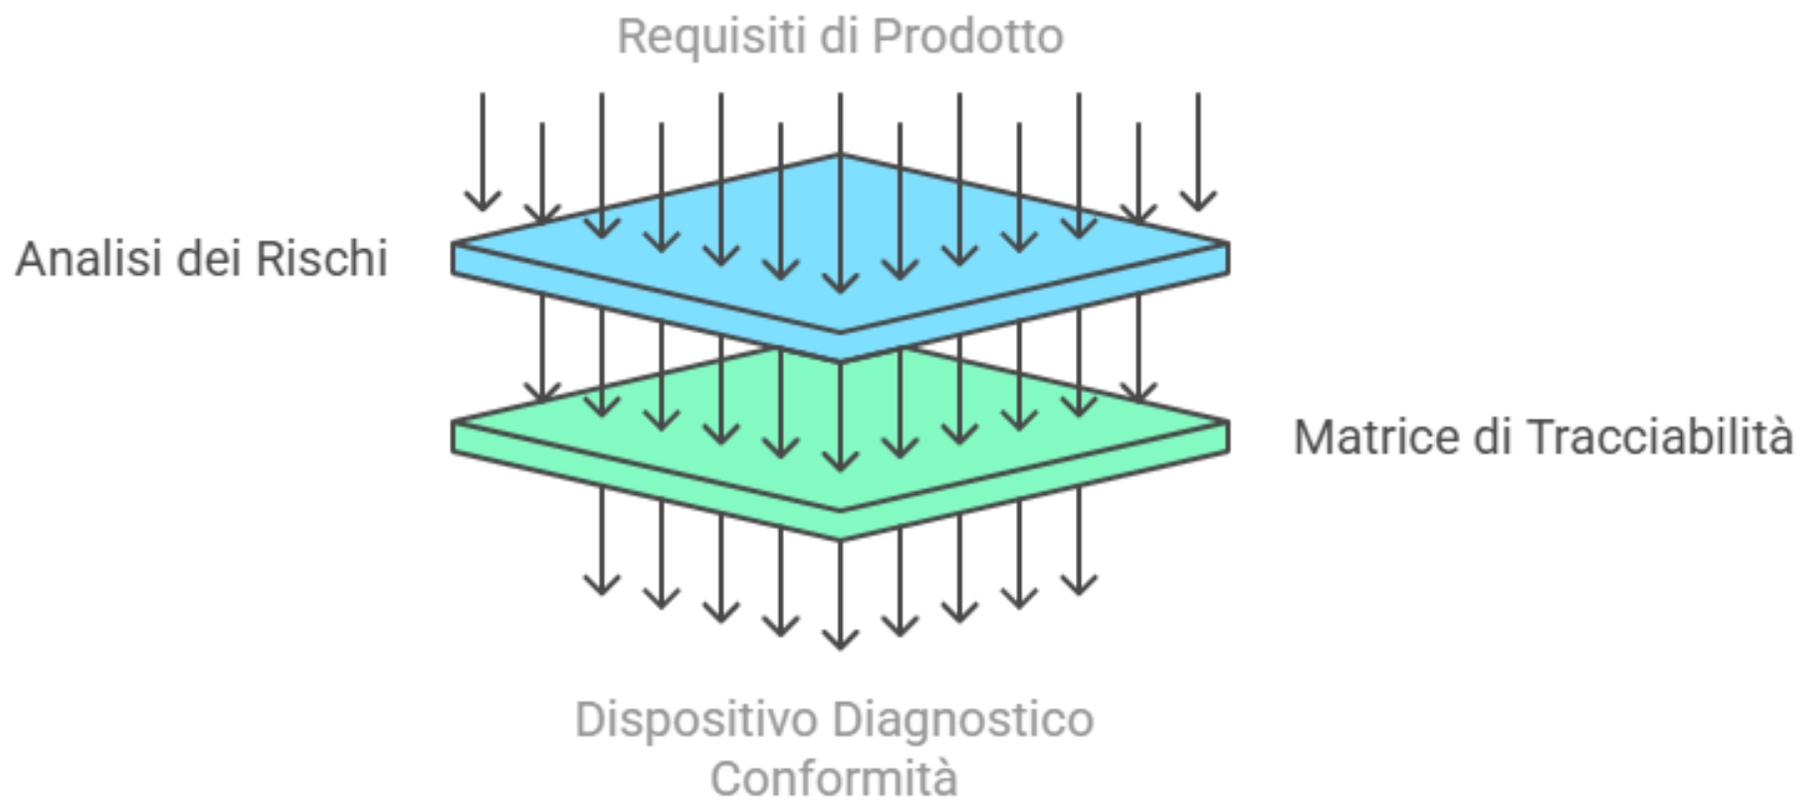

OTTENIMENTO DI UN PRODOTTO



PROSSIMO INCONTRO

(Coletta Giuliano)

*Test immunologici per applicazioni
POCT (basi teorico e metodologie di
sviluppo)*

